

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 07/23/2023

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:10
INTERNAL STANDARD	VERIFIED	09:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:10
BLANK TEST	0.00	09:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:12
BLANK TEST	0.00	09:13

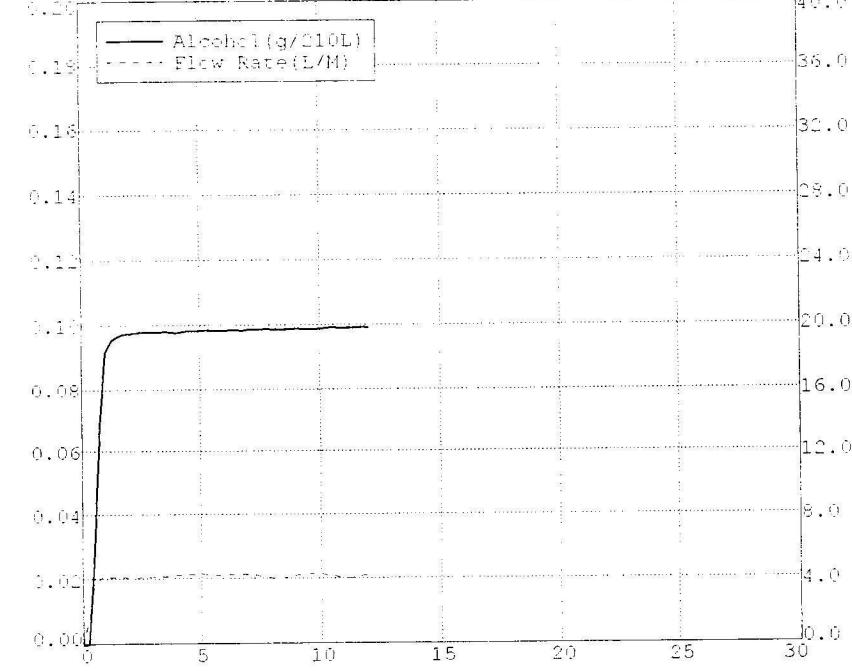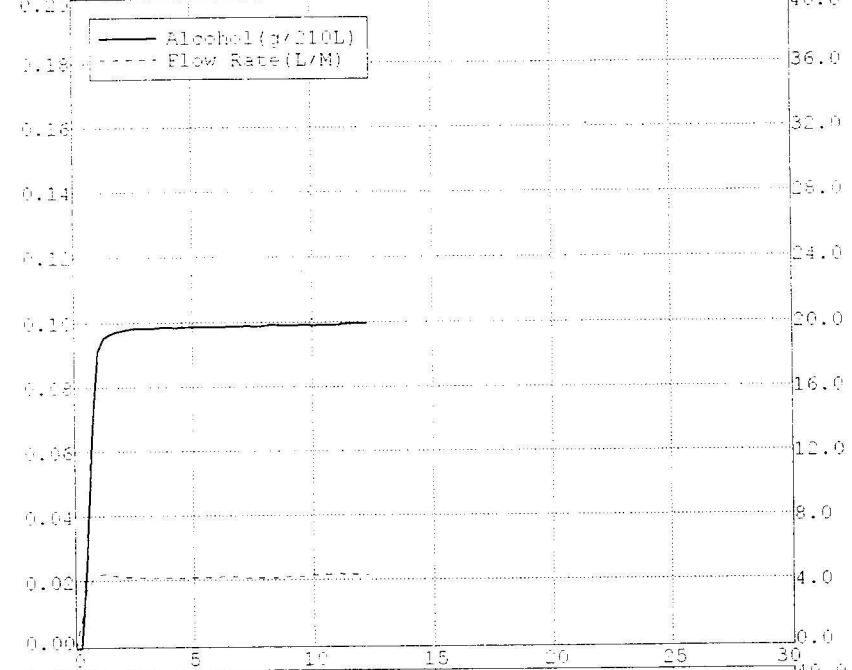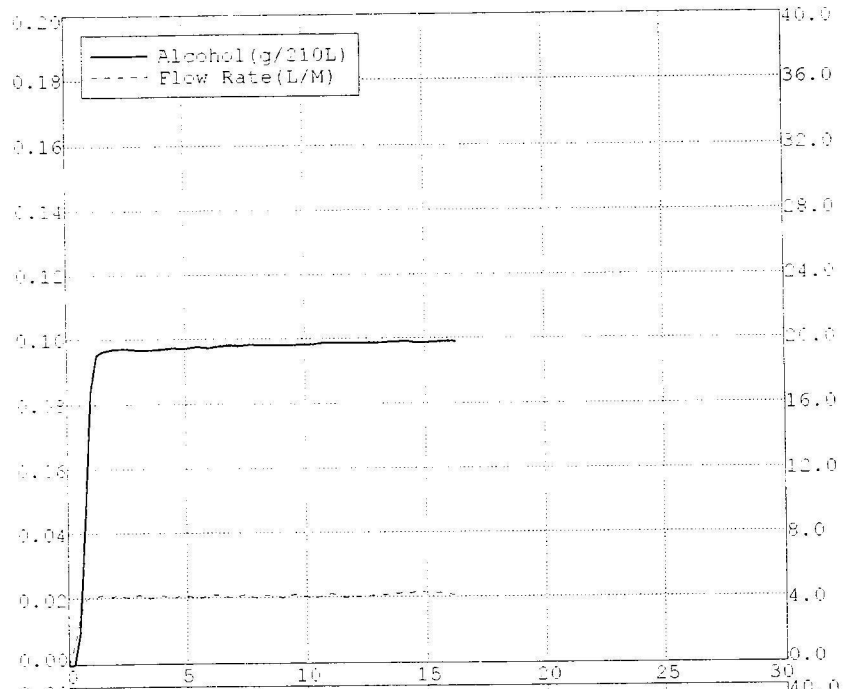

@614