

SUPERVISOR TEST




-----  
 SPRING VALLEY VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 127106  
 -----

Date: 08/15/2023

OPERATOR NAME:  
 BRANDON KING  
 Permit #: 36388  
 Operator Agency/Dept: SPRING VALLEY PD  
 Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:21
INTERNAL STANDARD	VERIFIED	00:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:23
BLANK TEST	0.00	00:24

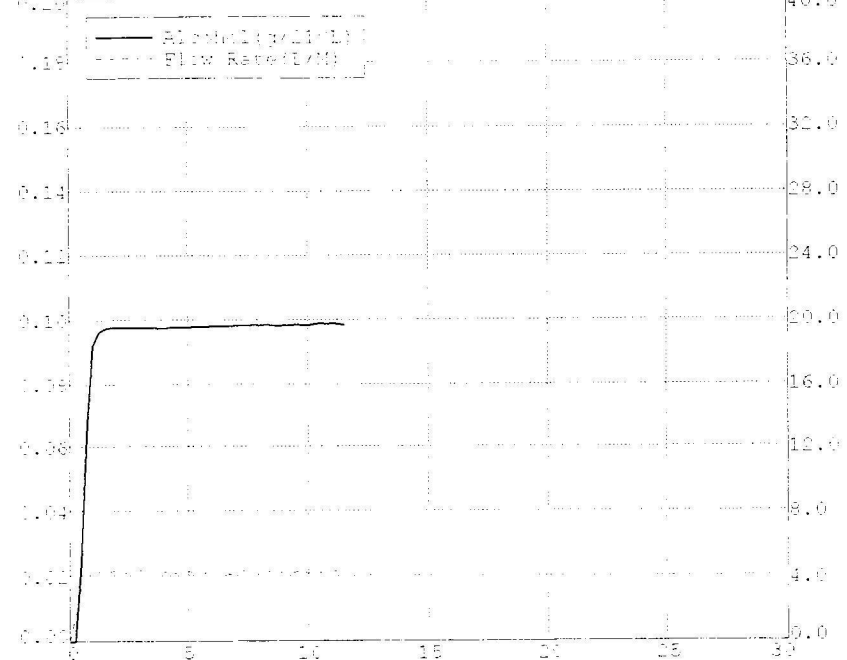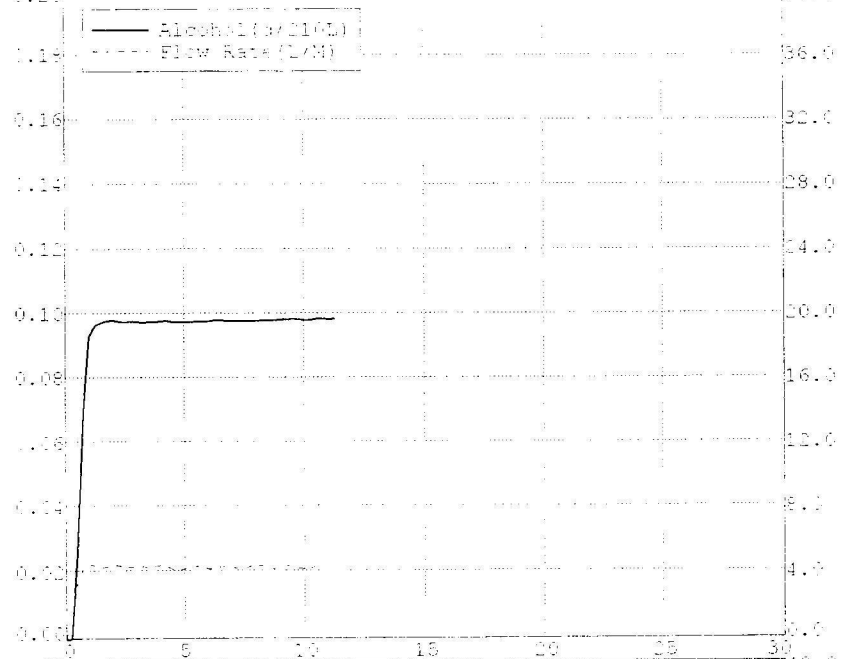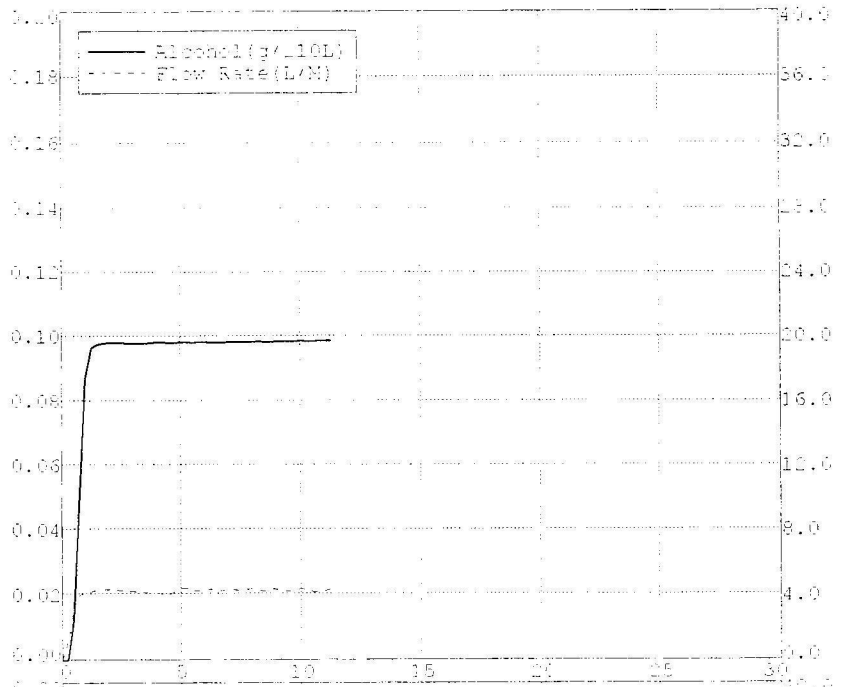

614