

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 09/13/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:56
INTERNAL STANDARD	VERIFIED	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:57
BLANK TEST	0.00	16:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:58
BLANK TEST	0.00	16:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:59
BLANK TEST	0.00	17:00

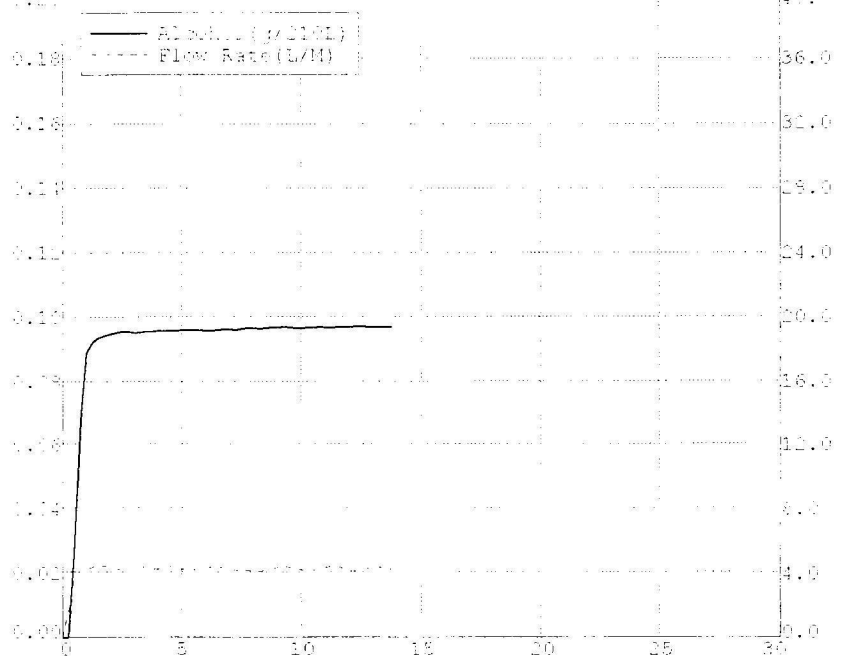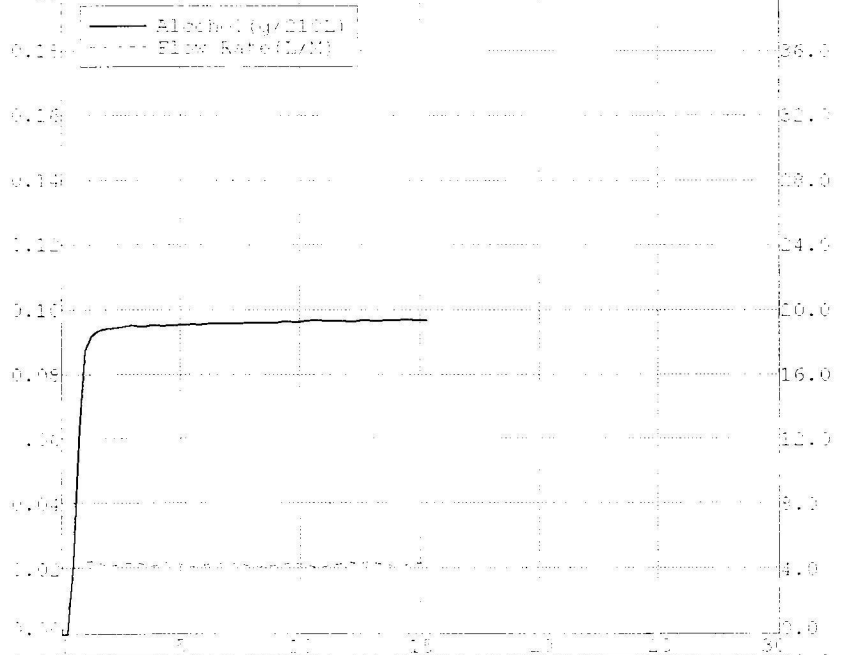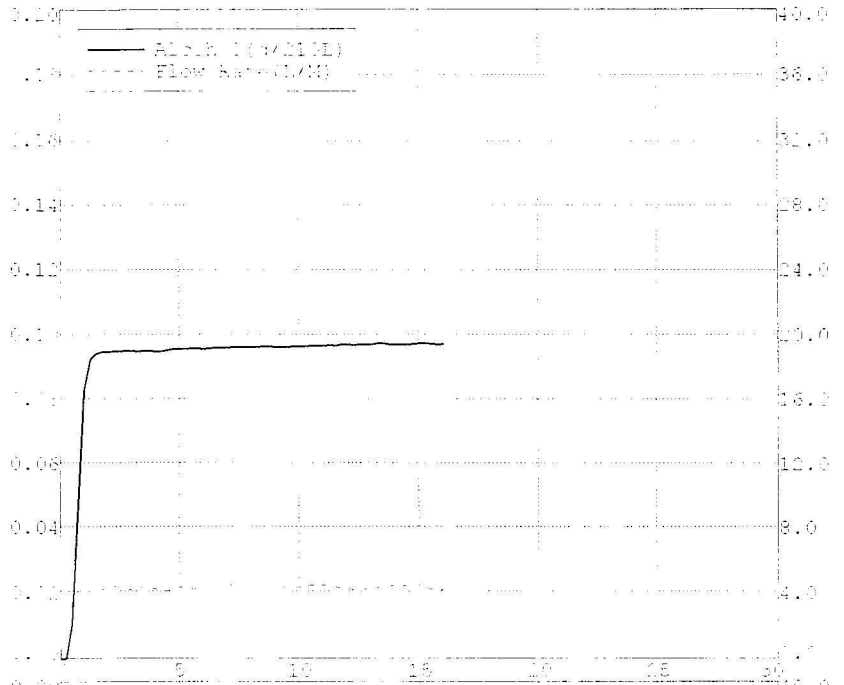

Handwritten signature and number 614