

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 09/29/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:20
INTERNAL STANDARD	VERIFIED	16:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:20
BLANK TEST	0.00	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:21
BLANK TEST	0.00	16:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:23
BLANK TEST	0.00	16:23

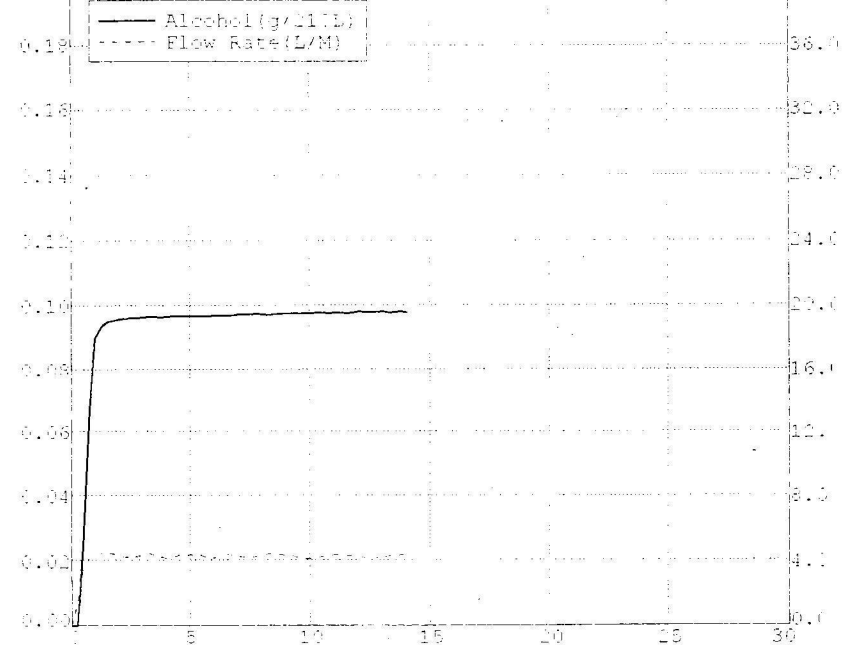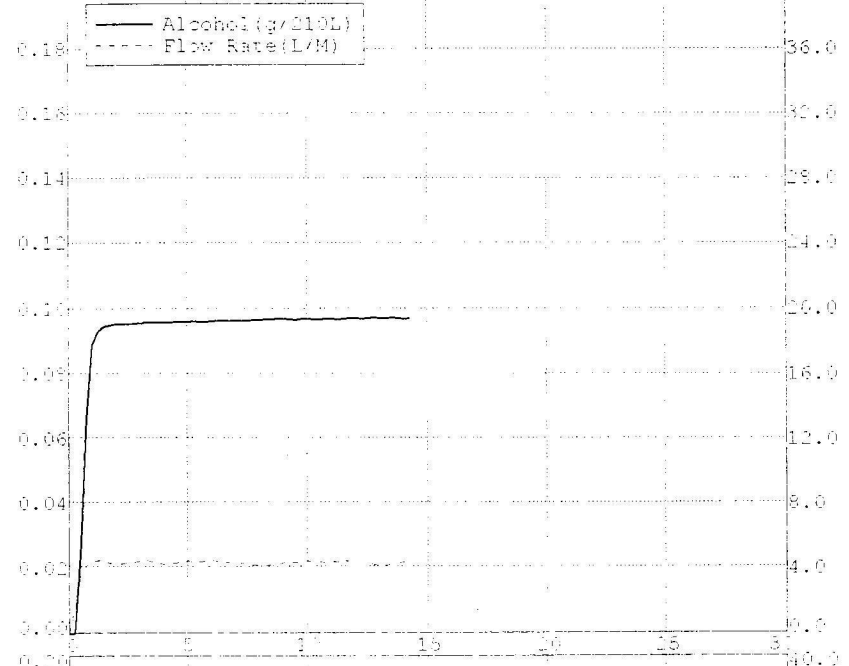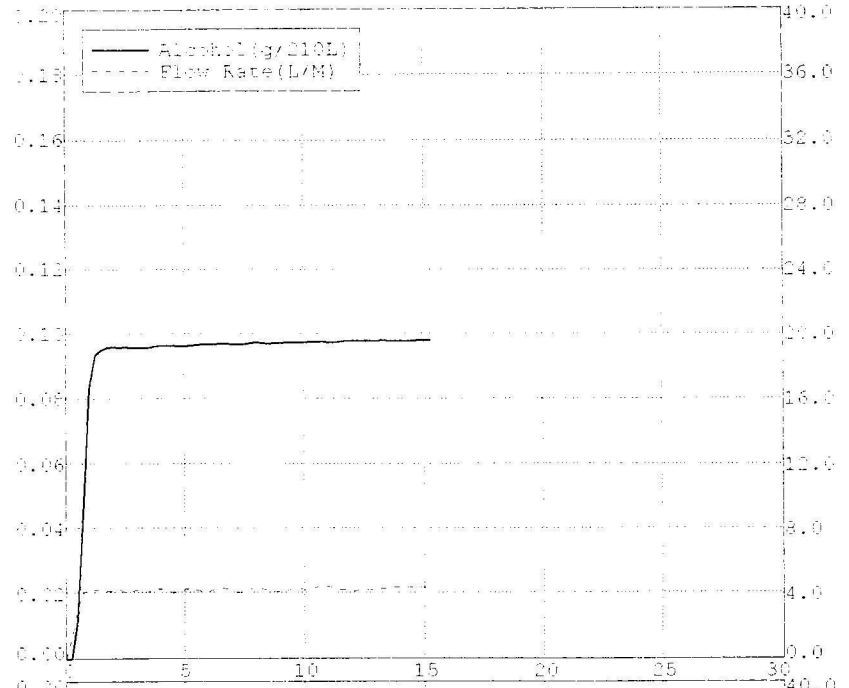

2614