

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 10/08/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:31
INTERNAL STANDARD	VERIFIED	08:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:32
BLANK TEST	0.00	08:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:33
BLANK TEST	0.00	08:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:34
BLANK TEST	0.00	08:35

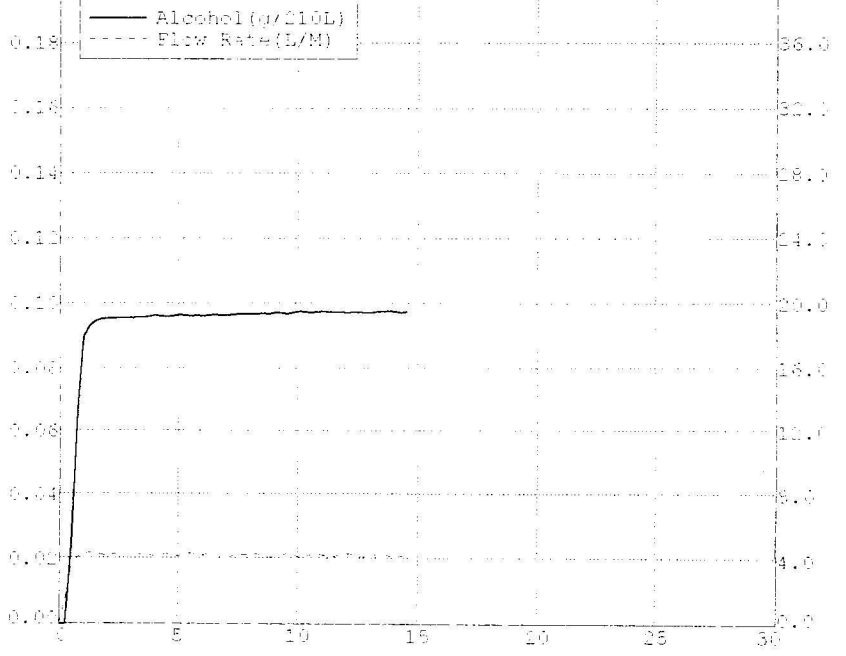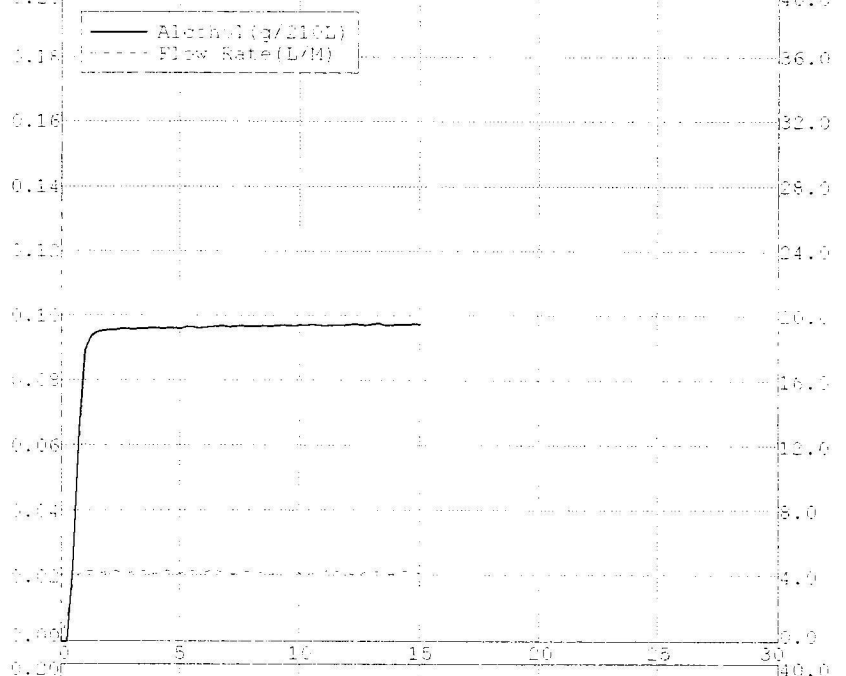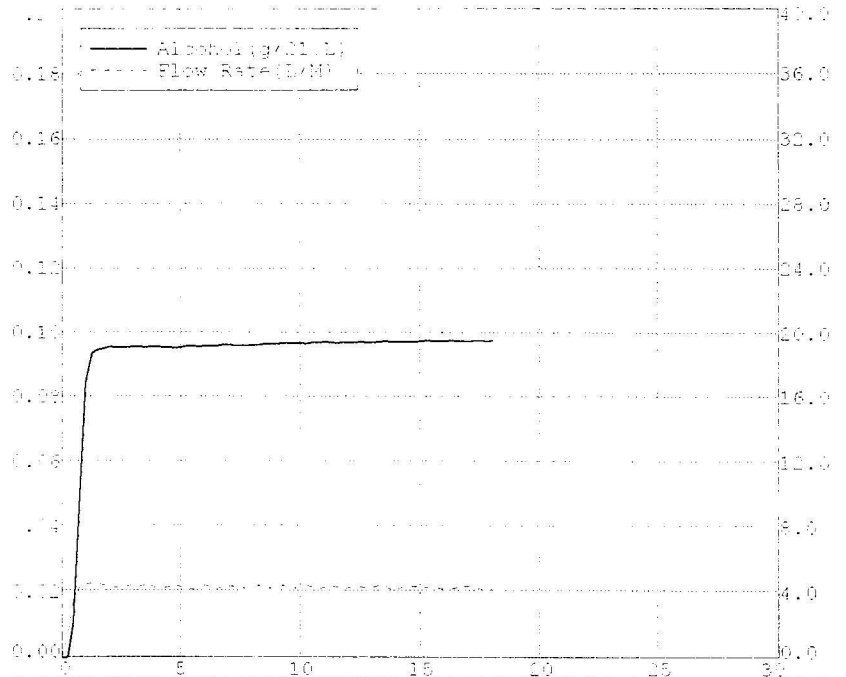

2614