

SUPERVISOR TEST




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 10/14/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:21
INTERNAL STANDARD	VERIFIED	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:23
BLANK TEST	0.00	16:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:24
BLANK TEST	0.00	16:25

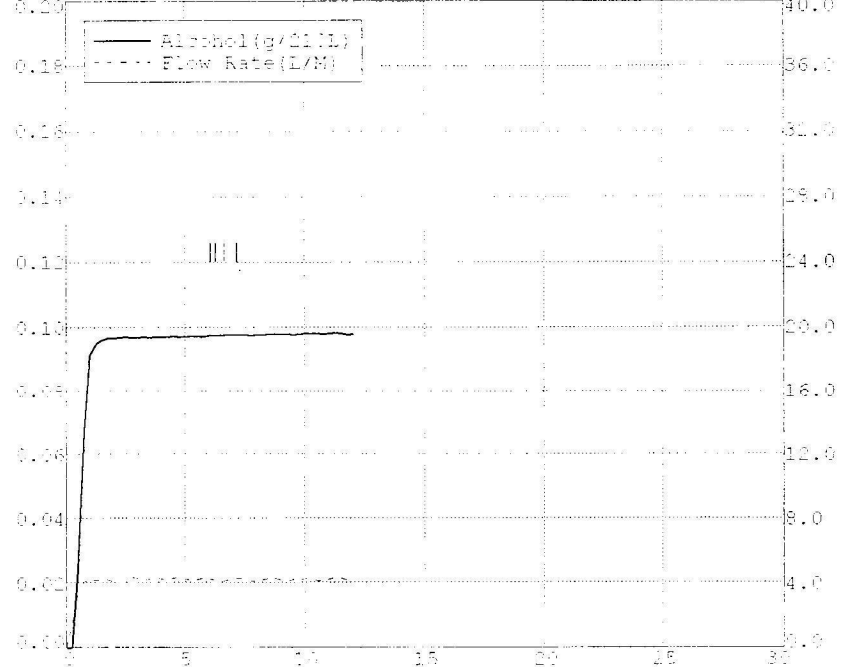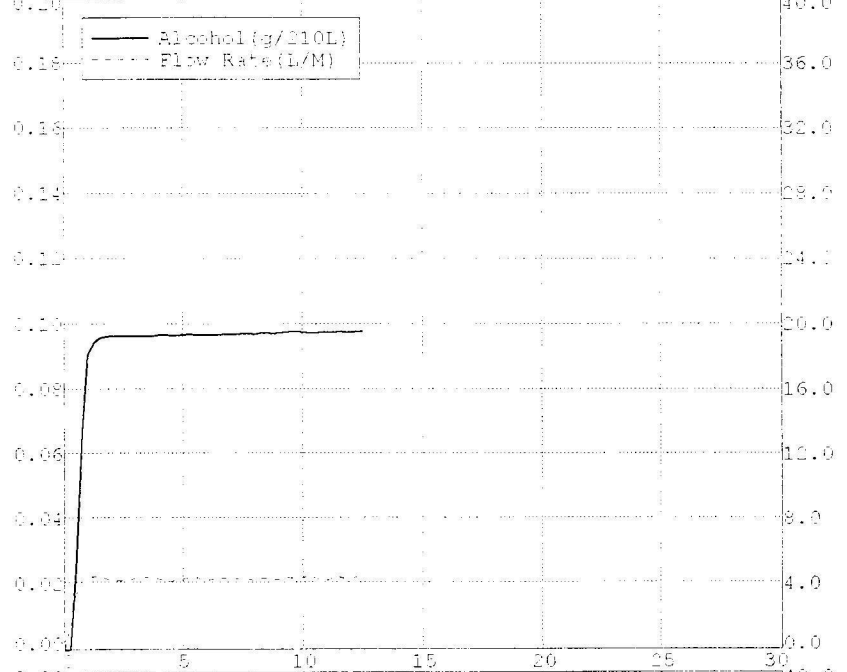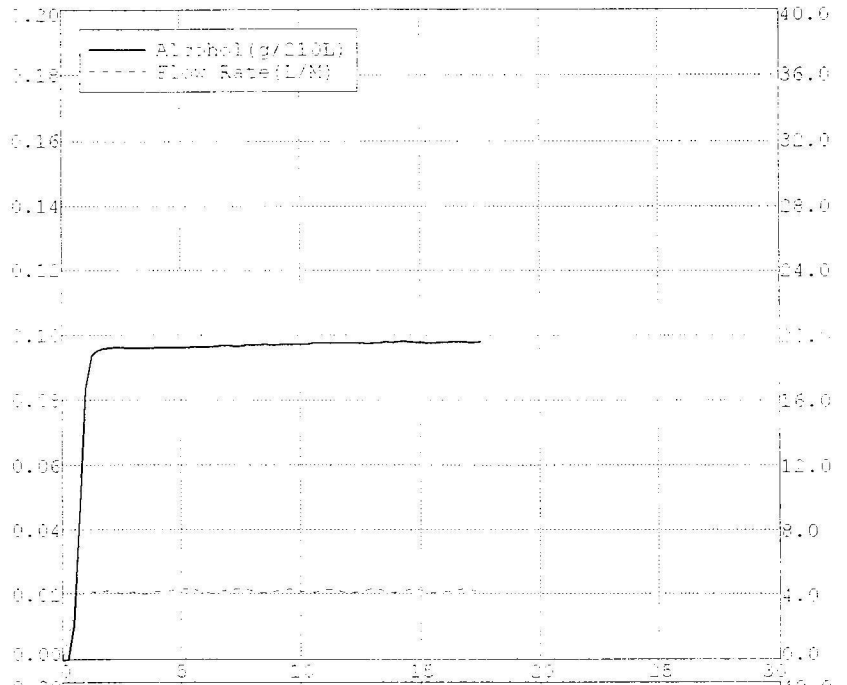

614