

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 11/05/2023

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:35
INTERNAL STANDARD	VERIFIED	10:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:38
BLANK TEST	0.00	10:39

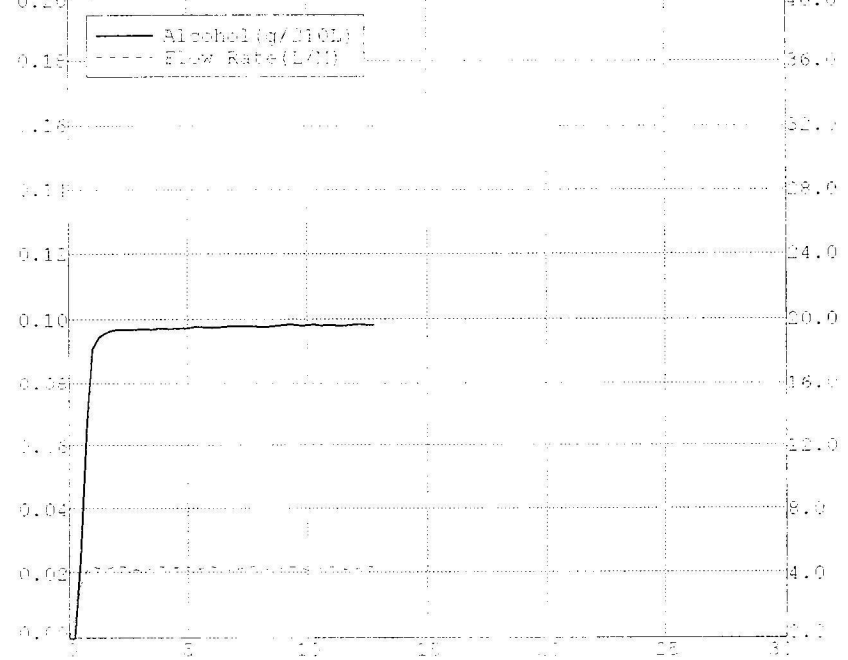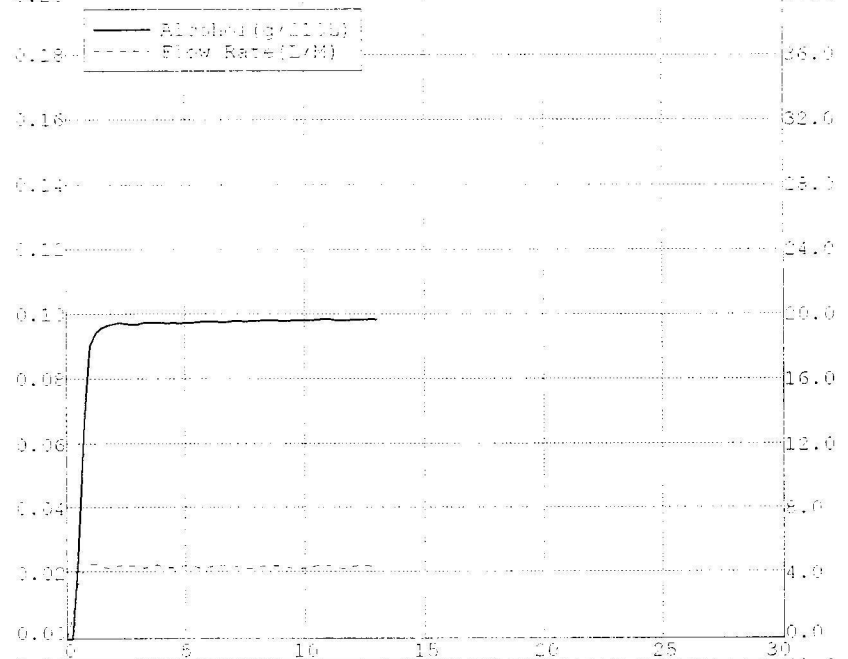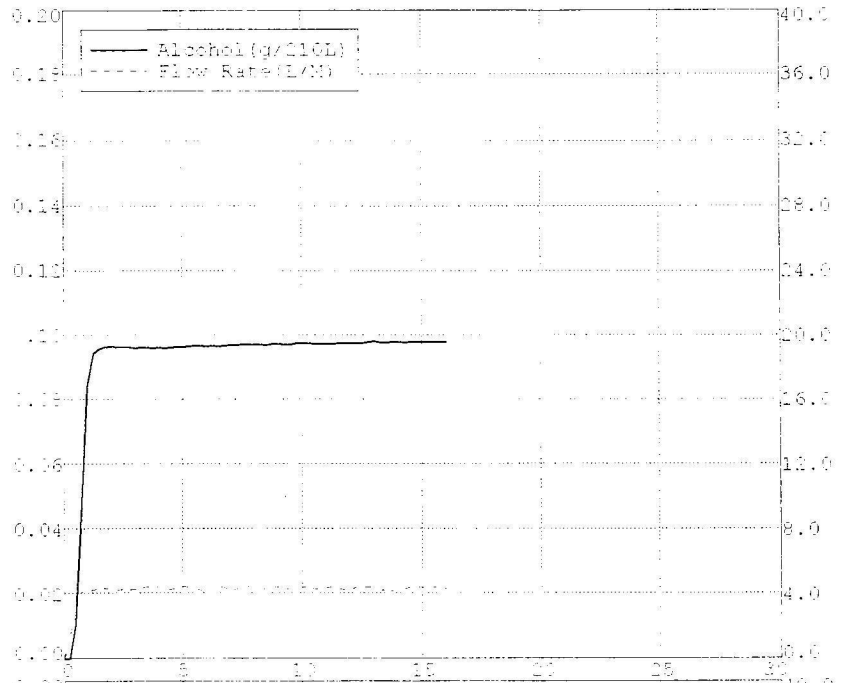

614