

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 12/24/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:32
INTERNAL STANDARD	VERIFIED	08:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:33
BLANK TEST	0.00	08:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:34
BLANK TEST	0.00	08:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:35
BLANK TEST	0.00	08:36

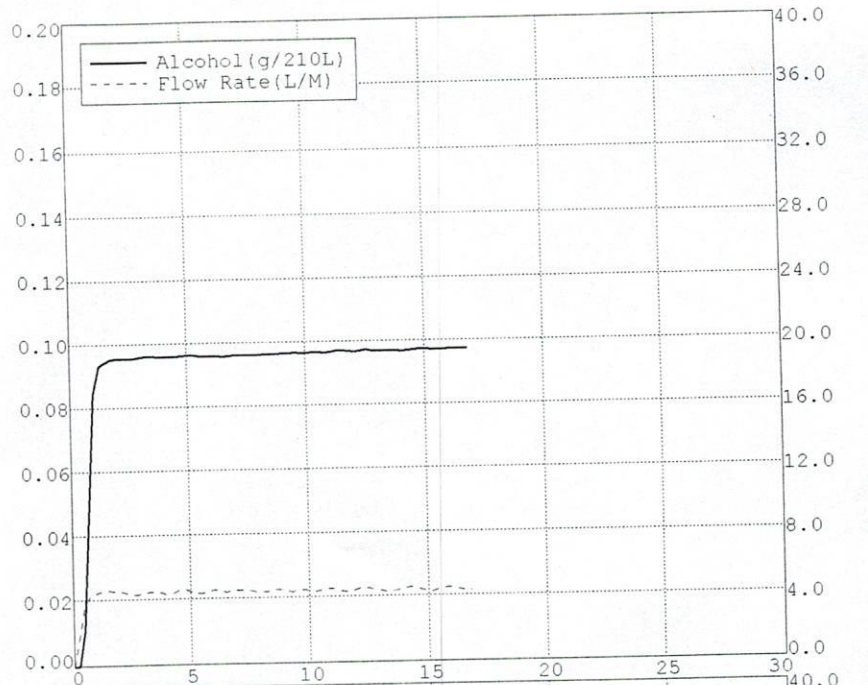

0614