

SUPERVISOR TEST



-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 12/30/2023

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:29
INTERNAL STANDARD	VERIFIED	16:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:30
BLANK TEST	0.00	16:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:31
BLANK TEST	0.00	16:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:32
BLANK TEST	0.00	16:33

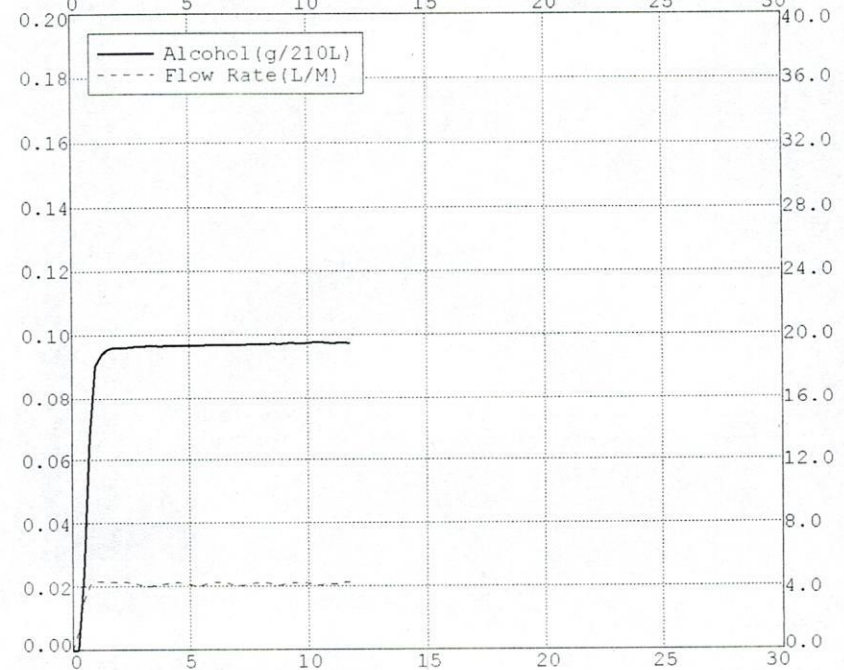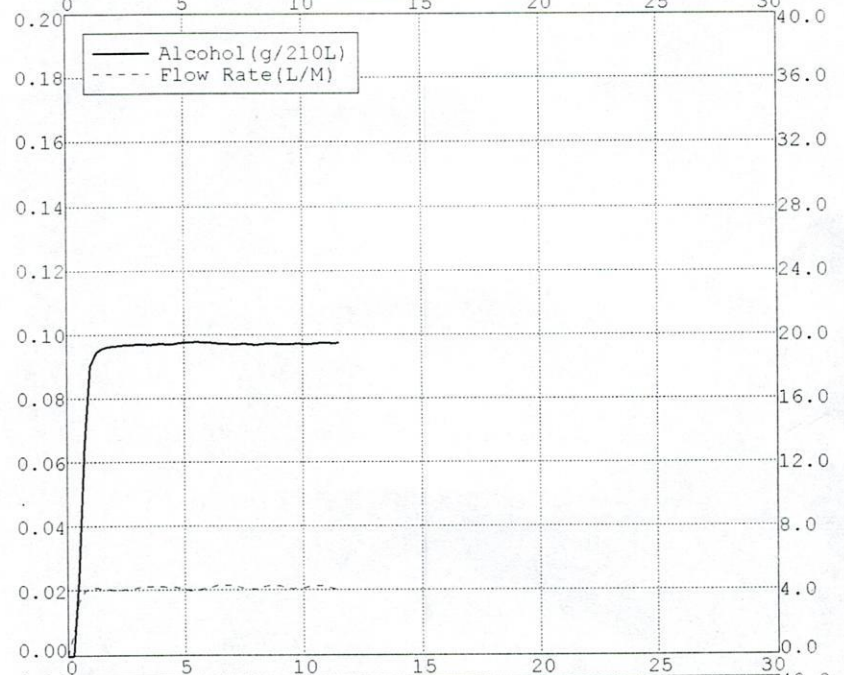

*Handwritten signature: B. King*