

SUPERVISOR TEST




 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 01/07/2024

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:33
INTERNAL STANDARD	VERIFIED	13:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:33
BLANK TEST	0.00	13:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:34
BLANK TEST	0.00	13:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:36
BLANK TEST	0.00	13:36

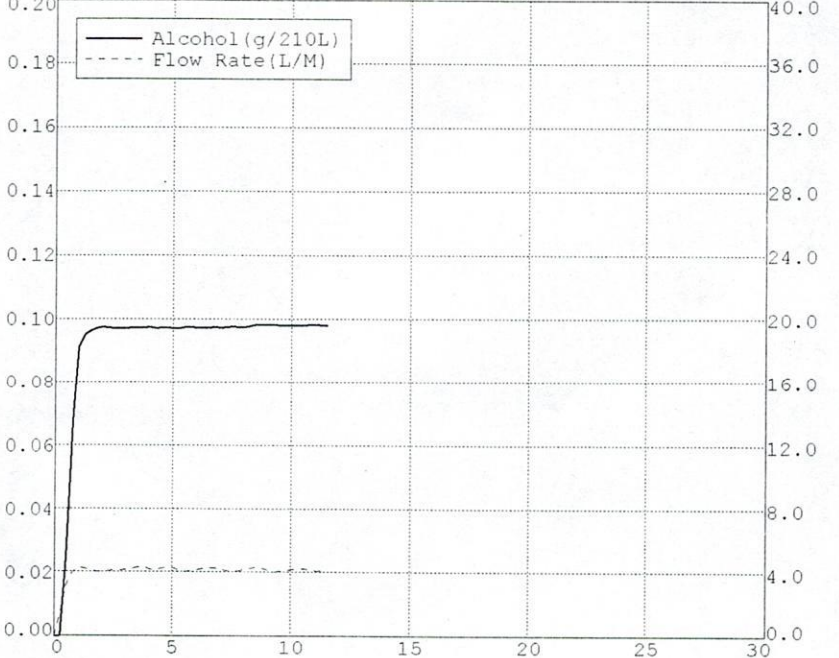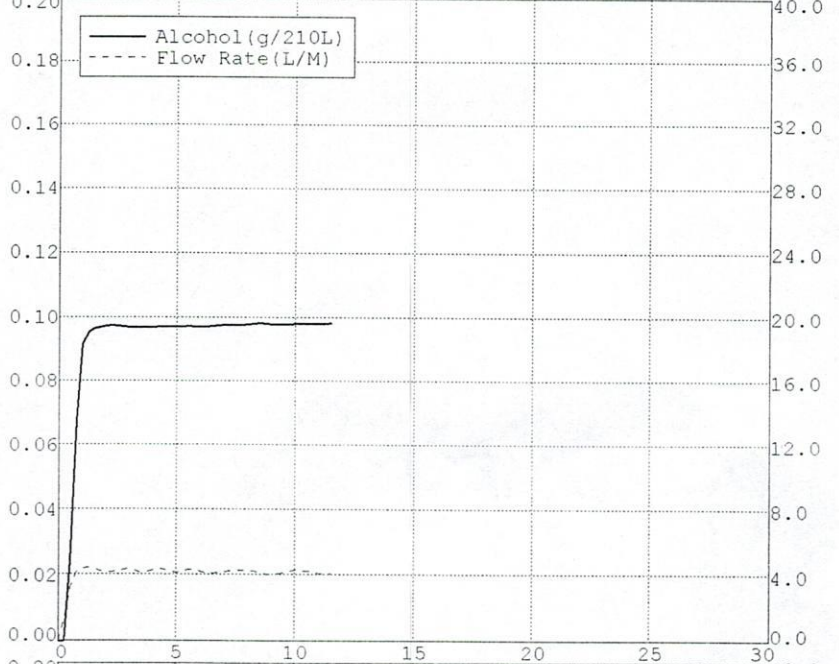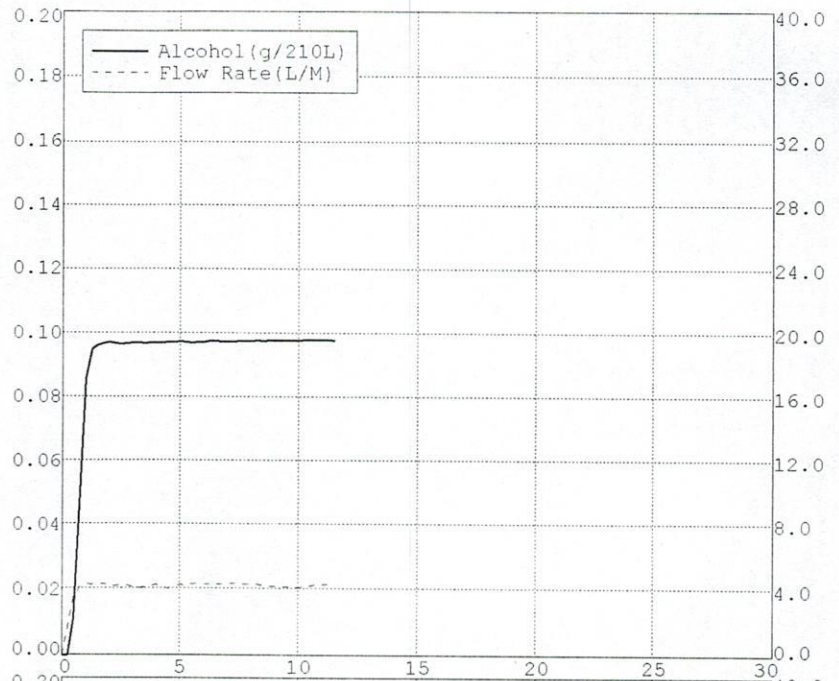

2614