

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 01/18/2024

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:23
INTERNAL STANDARD	VERIFIED	00:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27

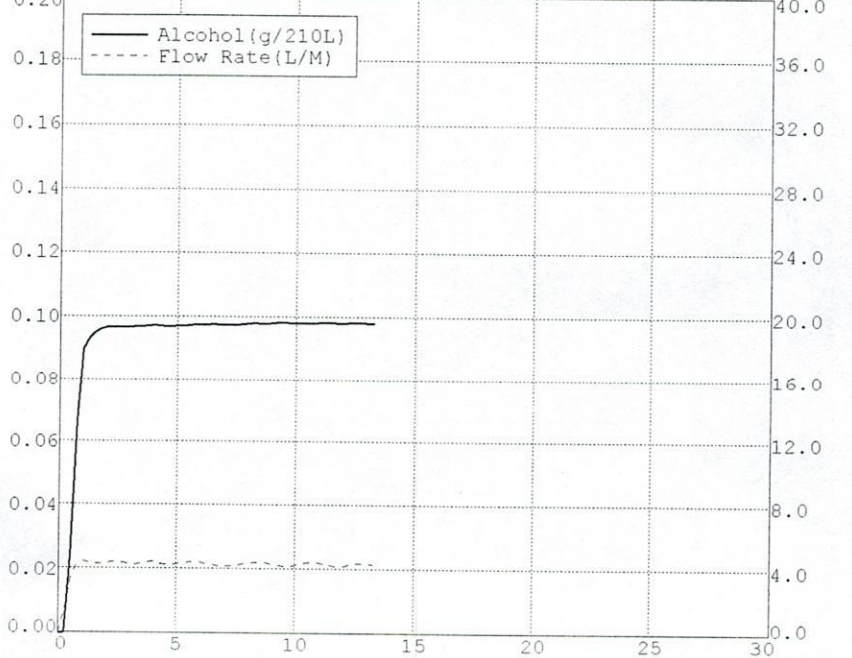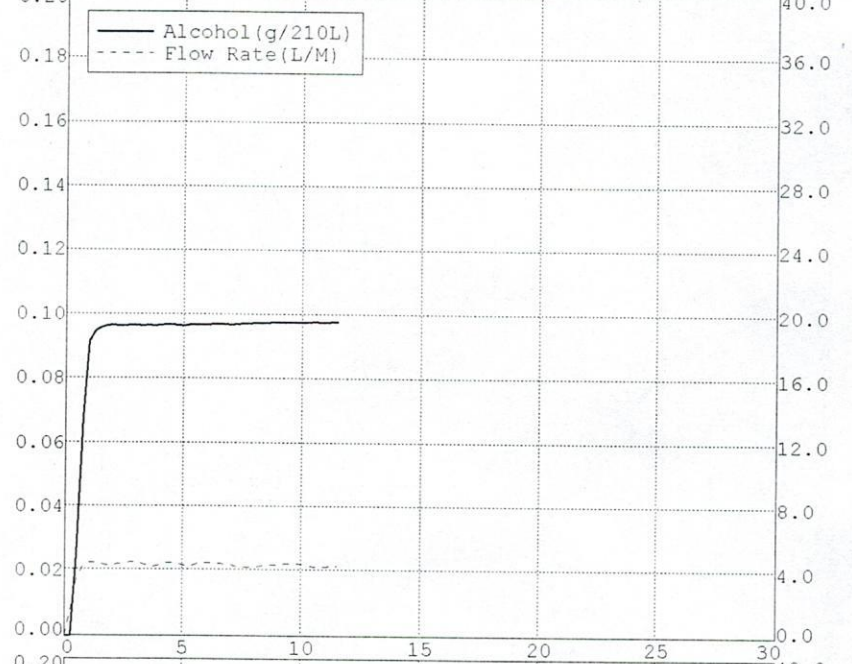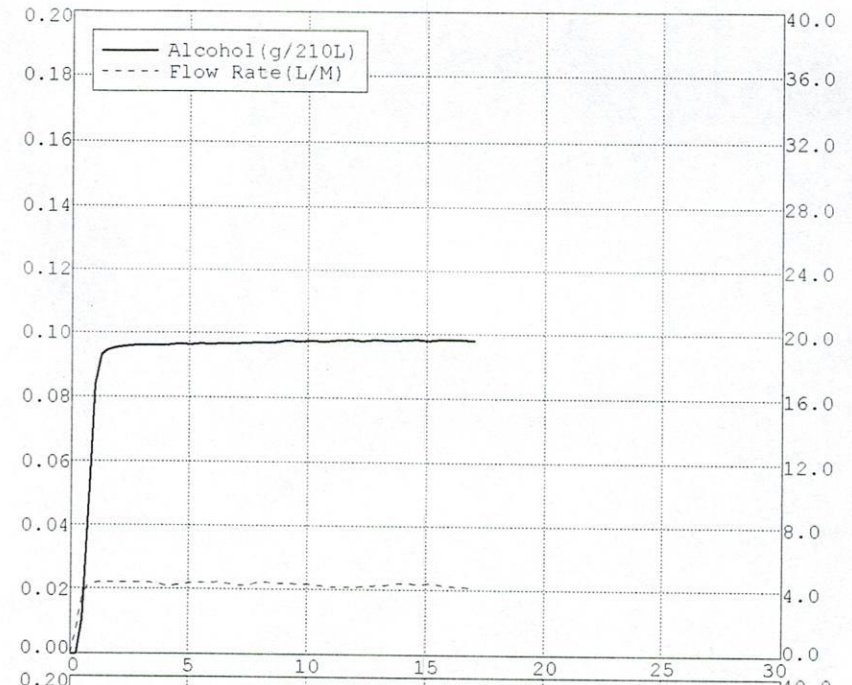

@614