

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 01/22/2024

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:38
BLANK TEST	0.00	00:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:41

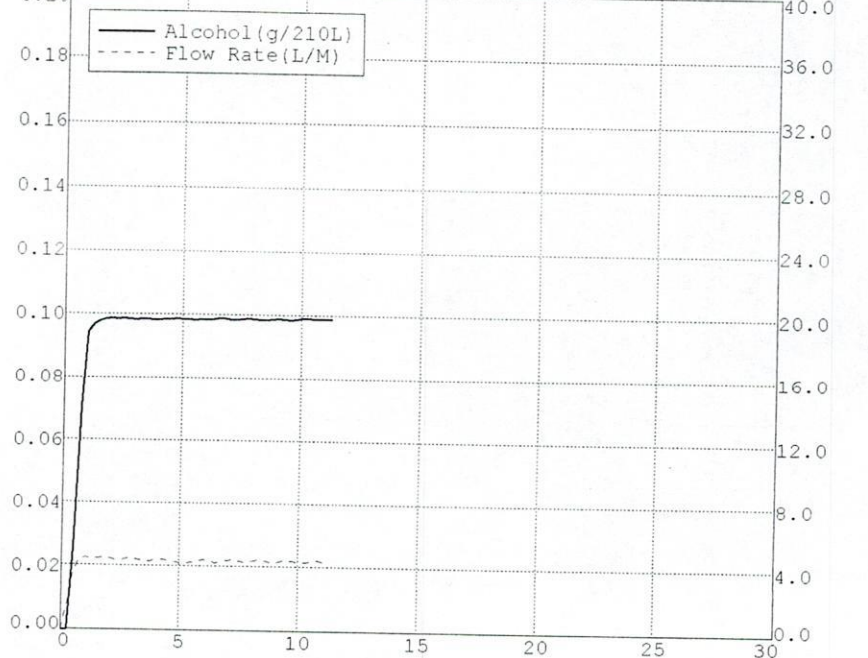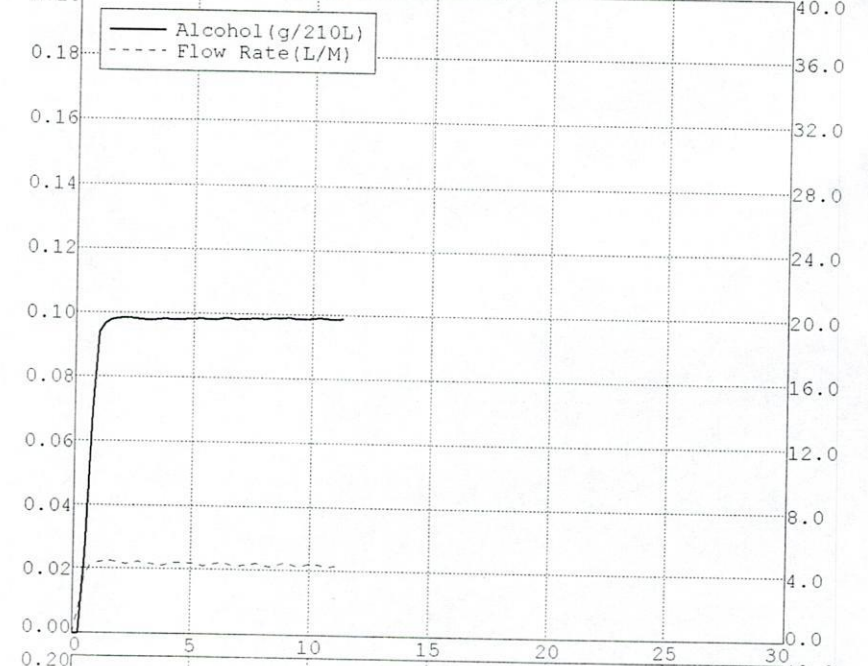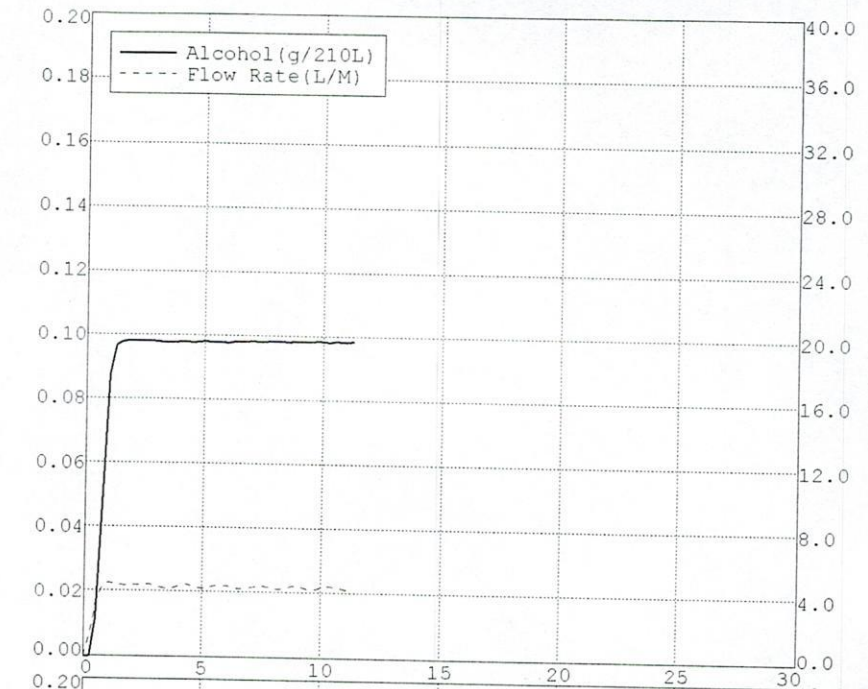

0614