

SOLUTION CHANGE

 SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 02/07/2024

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:20
INTERNAL STANDARD	VERIFIED	07:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:21
BLANK TEST	0.00	07:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:23
BLANK TEST	0.00	07:24

ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

23430
LOT NO.




5/22/24
EXP. DATE

375
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
 A PROPERLY OPERATING BREATH SIMULATOR AND
 BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
 PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
 HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06

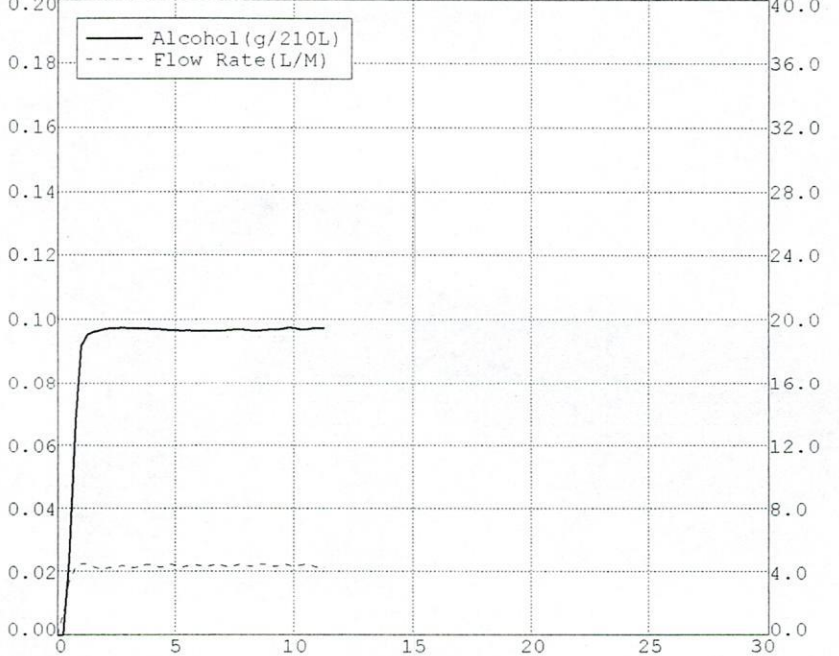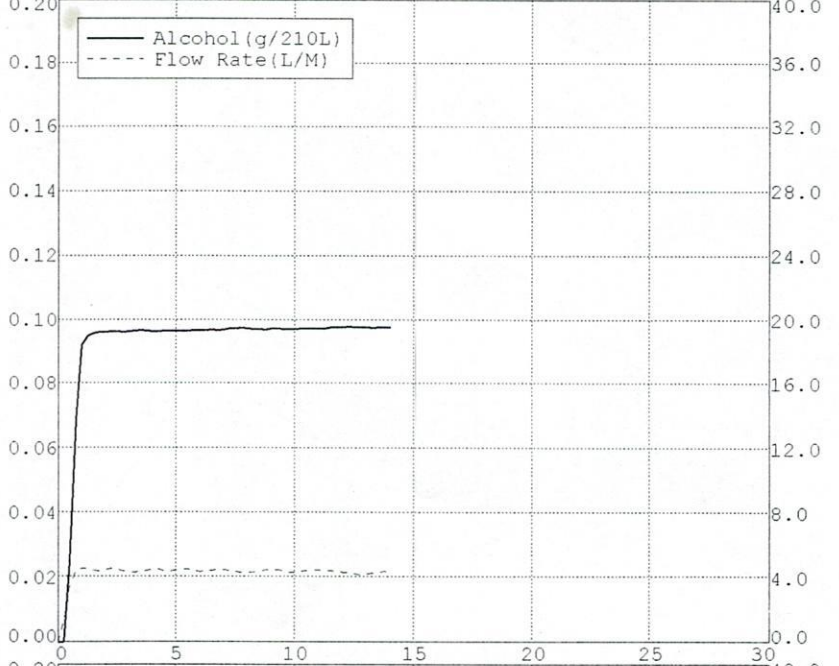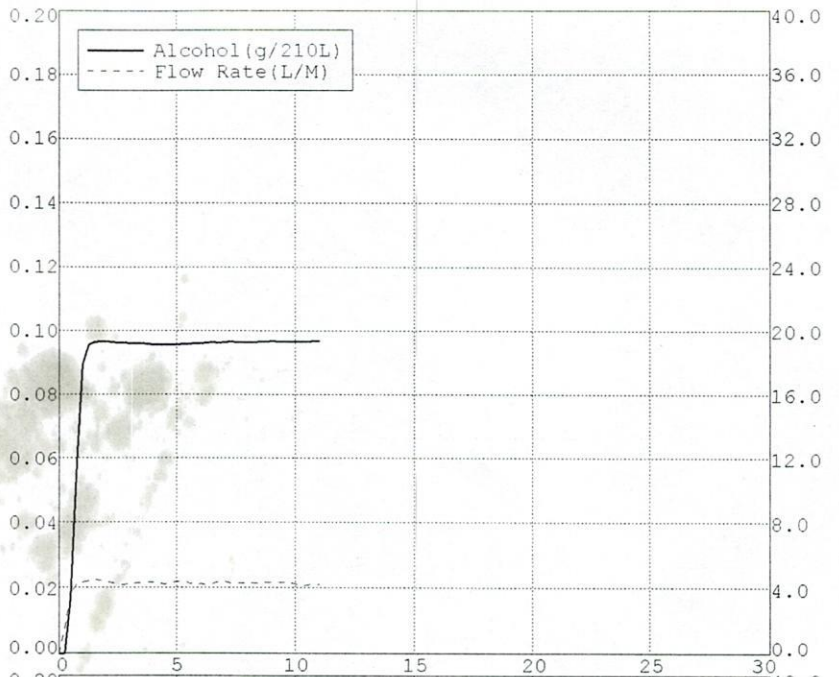

614