

SUPERVISOR TEST




-----  
SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106  
-----

Date: 02/13/2024

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:21
INTERNAL STANDARD	VERIFIED	01:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:21
BLANK TEST	0.00	01:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:24
BLANK TEST	0.00	01:25

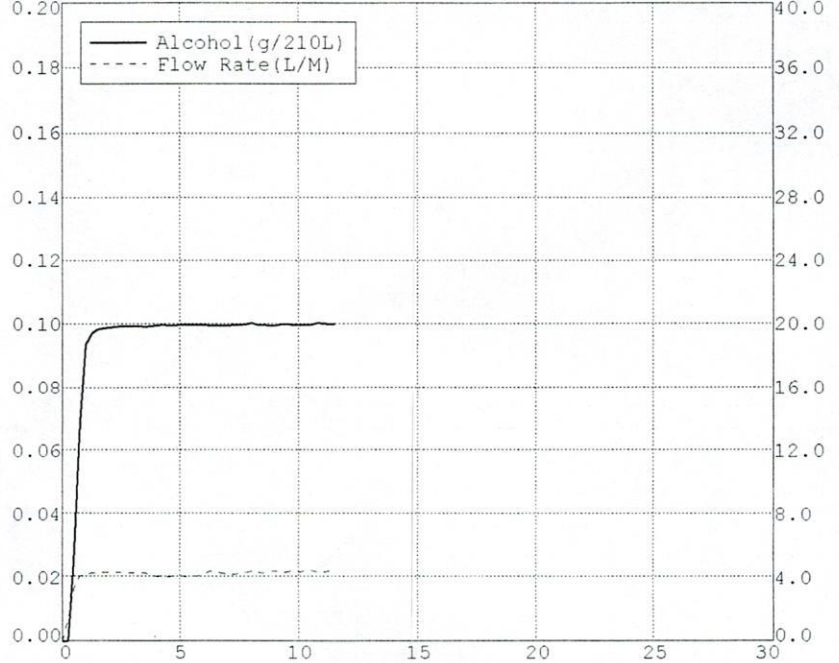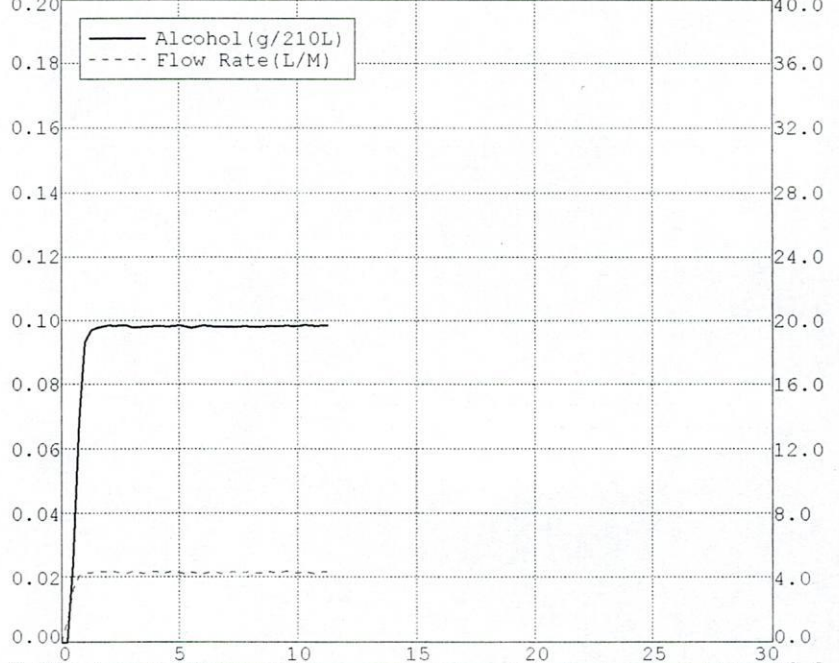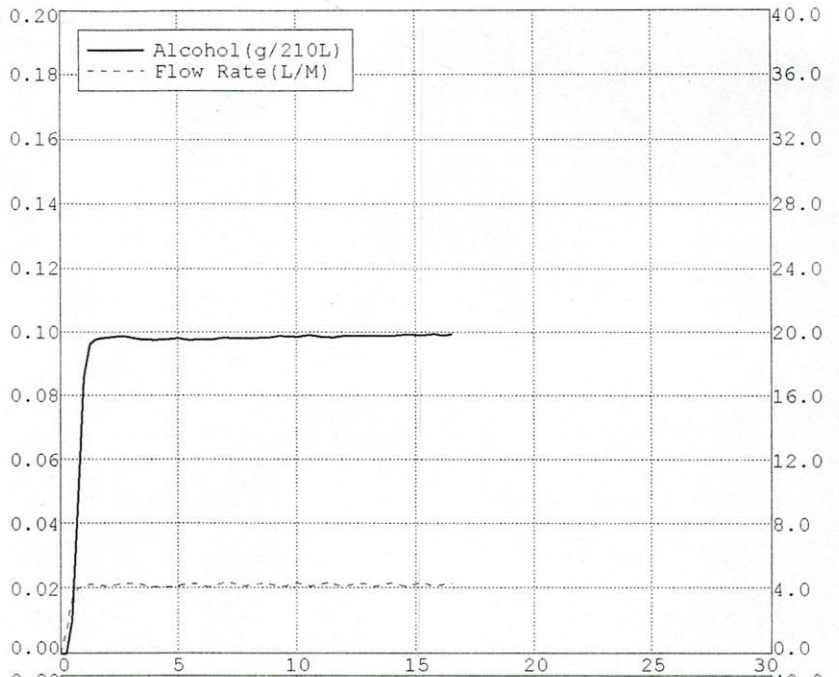

2614