

SOLUTION CHANGE




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 03/01/2024

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23430

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 07:59 |
| INTERNAL STANDARD | VERIFIED | 07:59 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:00 |
| BLANK TEST | 0.00 | 08:01 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:01 |
| BLANK TEST | 0.00 | 08:02 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:02 |
| BLANK TEST | 0.00 | 08:03 |

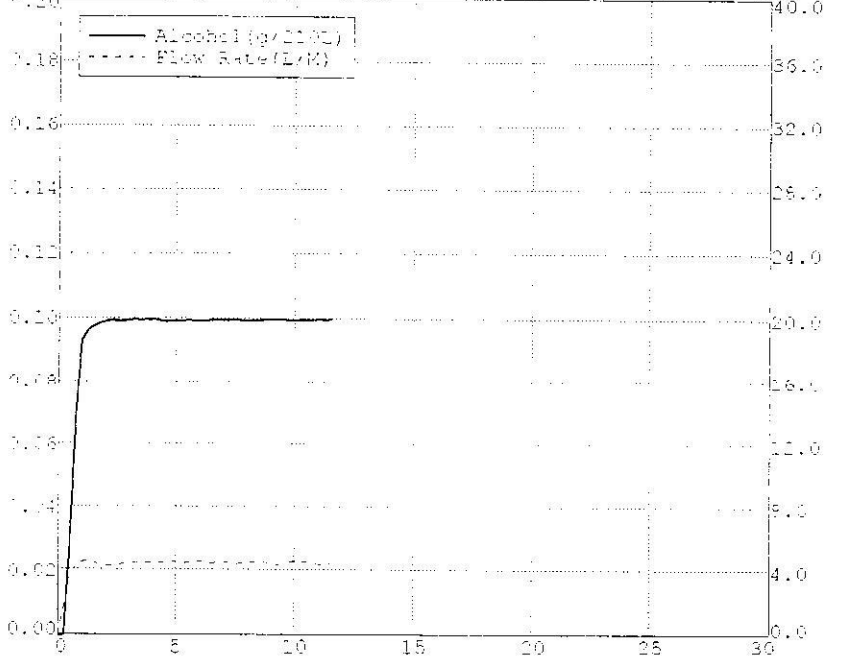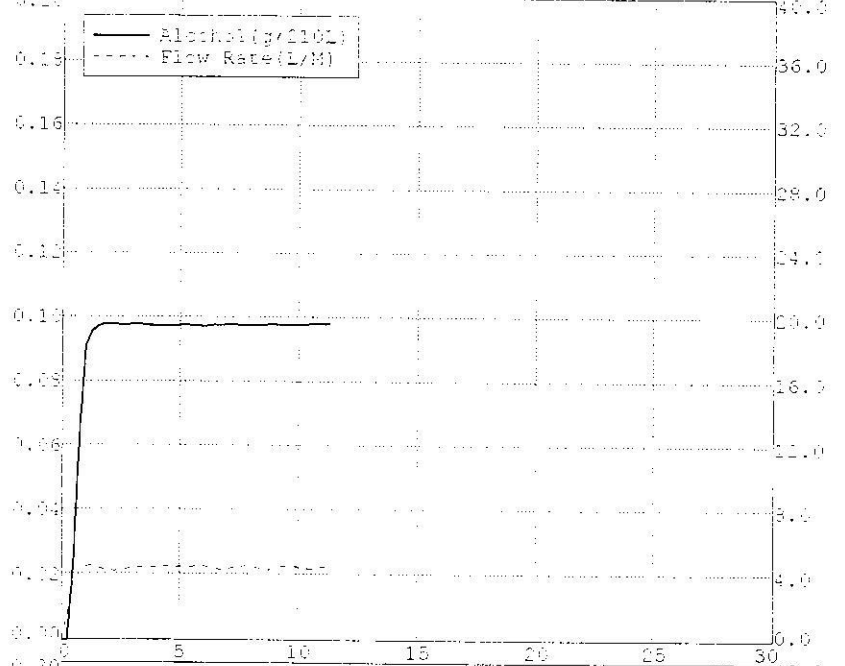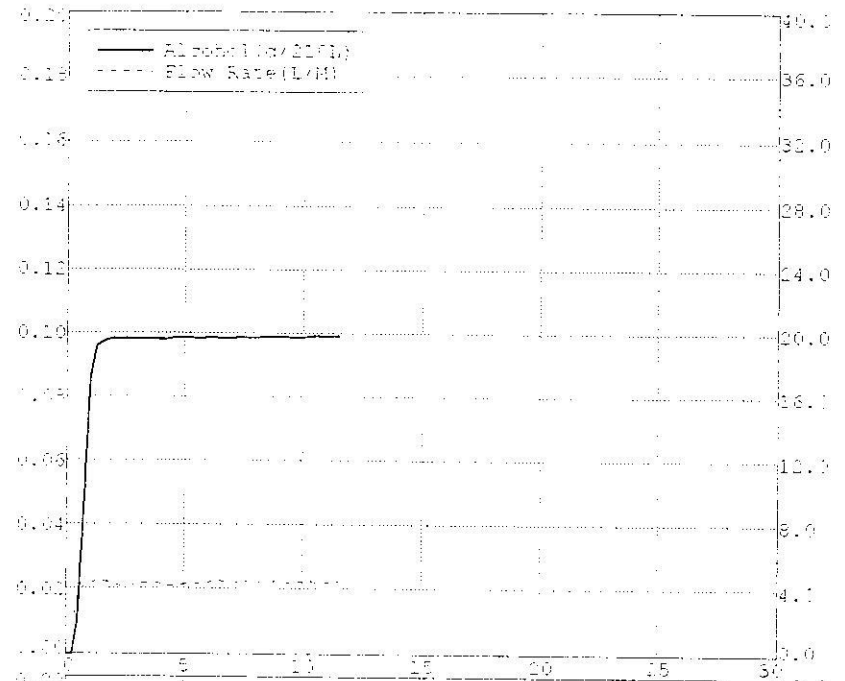

ALCOHOL REFERENCE SOLUTION
FOR SIMULATOR

23430
LOT NO.

5/22/24
EXP. DATE

388
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH
A PROPERLY OPERATING BREATH SIMULATOR AND
A BREATH ALCOHOL ANALYZER, THE SOLUTION WILL
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.
HARRISBURG, PENNSYLVANIA 17111

2024 01/06

2614