

SUPERVISOR TEST


SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 03/14/2024

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:29
INTERNAL STANDARD	VERIFIED	08:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:30
BLANK TEST	0.00	08:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:31
BLANK TEST	0.00	08:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:32
BLANK TEST	0.00	08:33

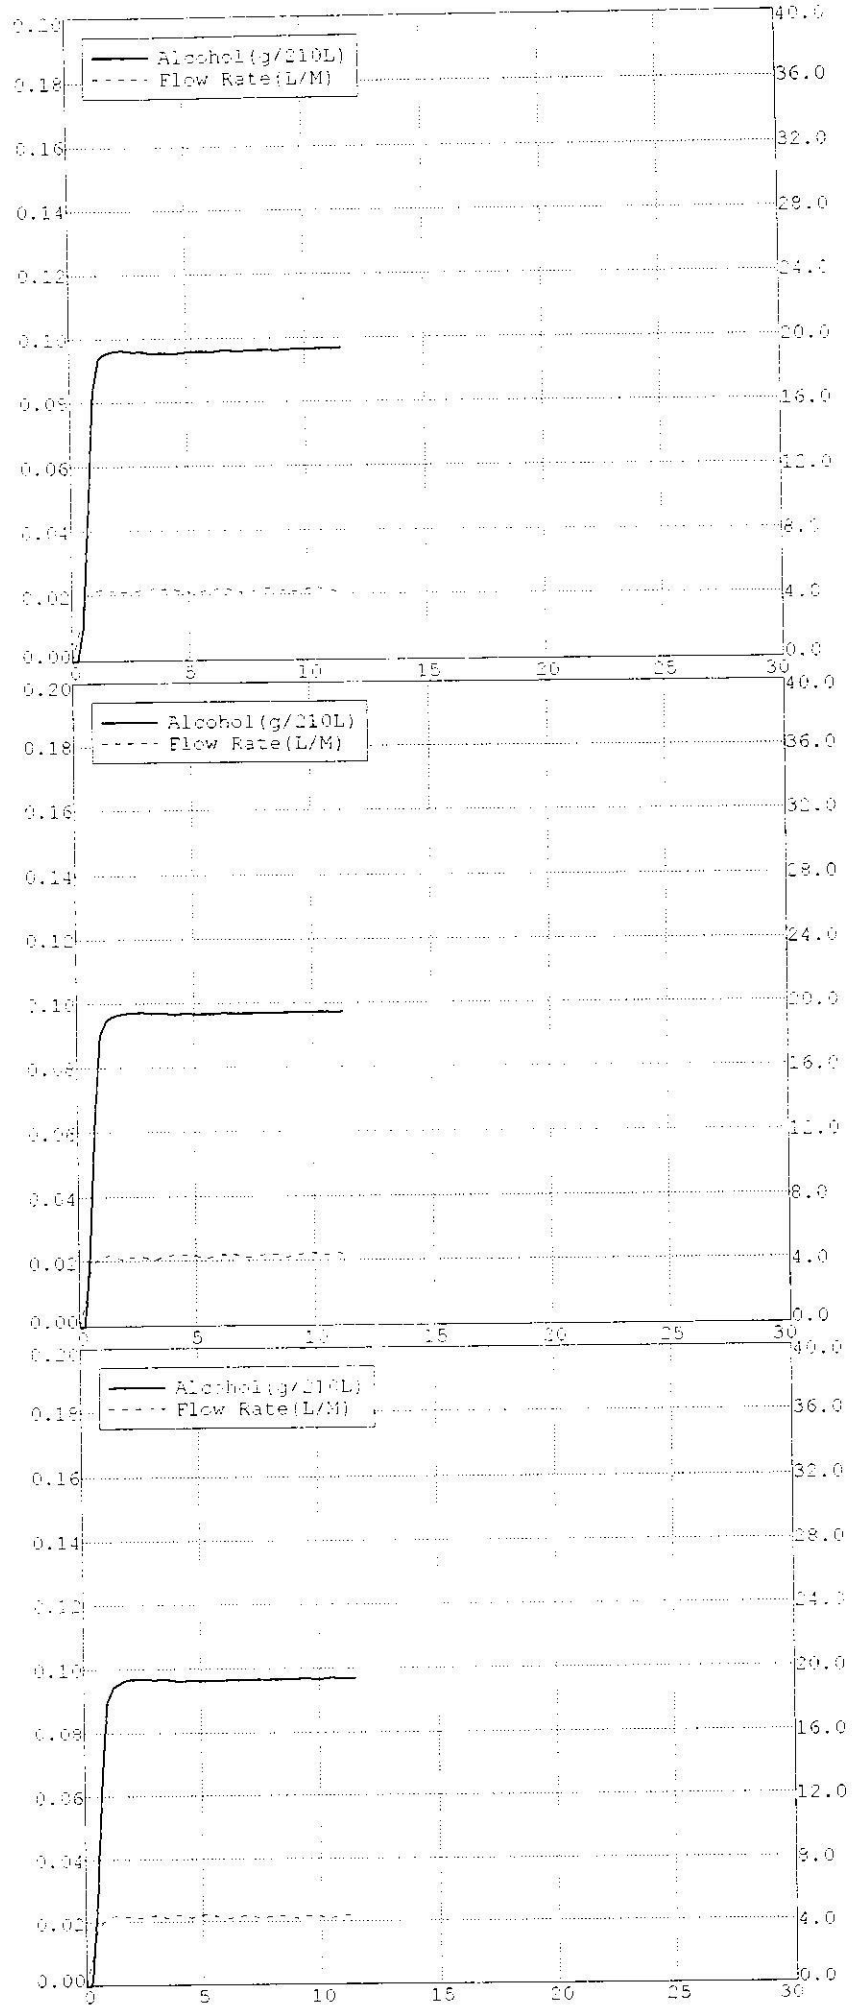

614