

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 04/05/2024

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:46
INTERNAL STANDARD	VERIFIED	00:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:47
BLANK TEST	0.00	00:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50

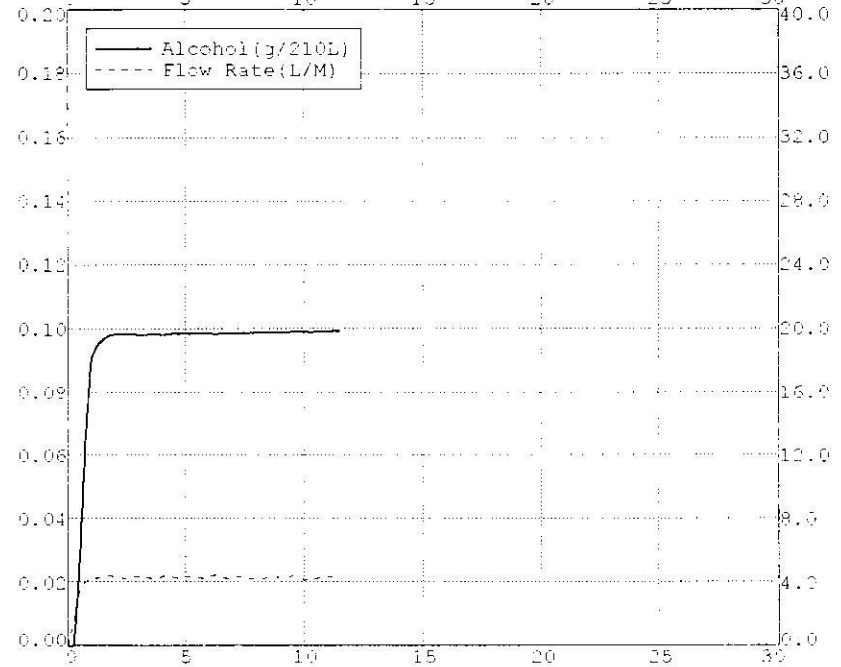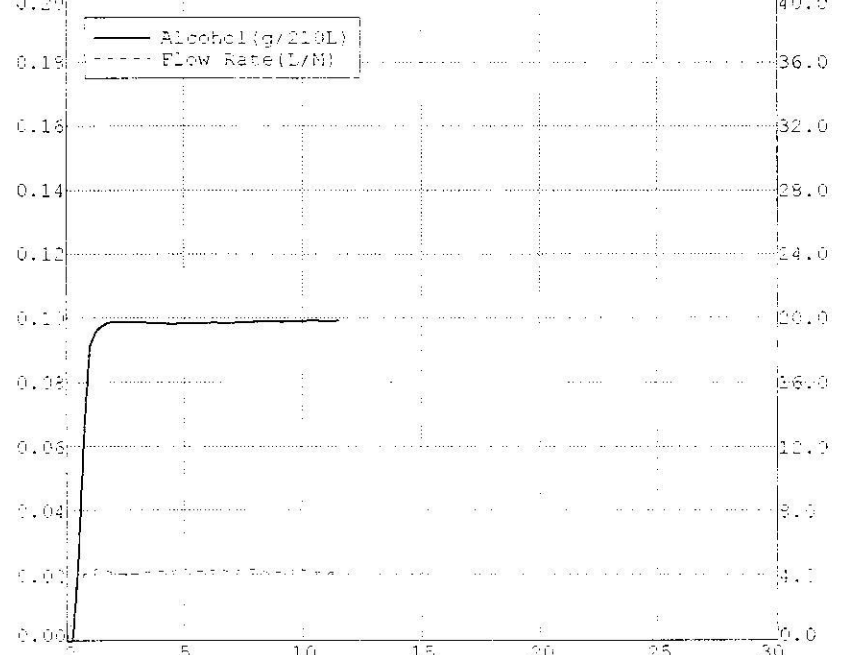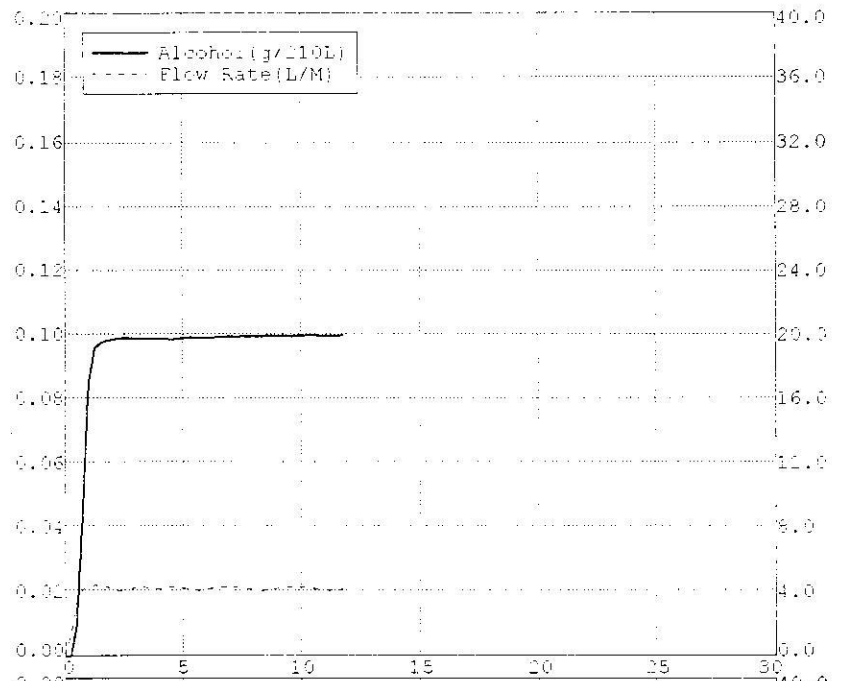

2614