

SUPERVISOR TEST




SPRING VALLEY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 127106

Date: 04/14/2024

OPERATOR NAME:
 BRANDON KING
 Permit #: 36388
 Operator Agency/Dept: SPRING VALLEY PD
 Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:38
INTERNAL STANDARD	VERIFIED	01:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:38
BLANK TEST	0.00	01:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:39
BLANK TEST	0.00	01:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:41
BLANK TEST	0.00	01:42

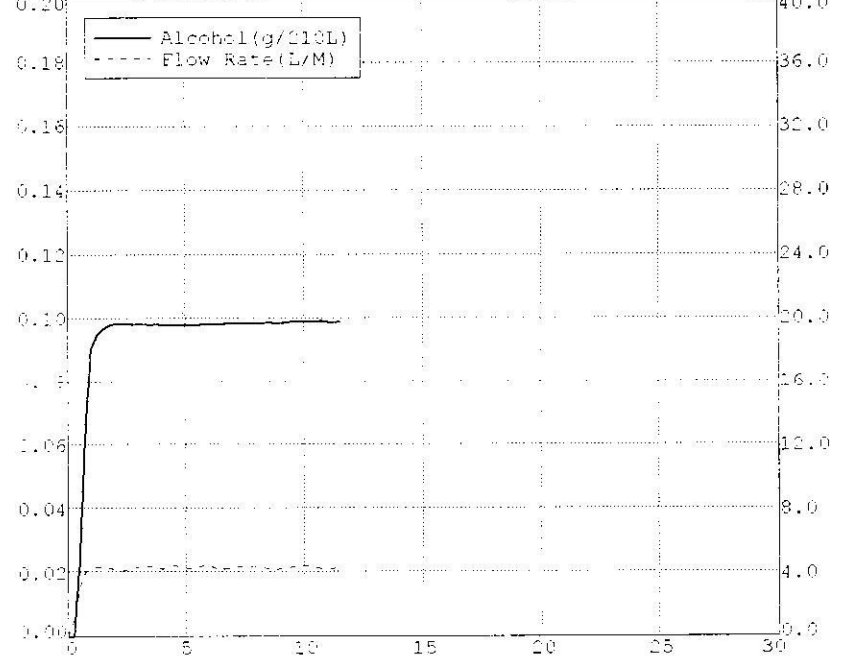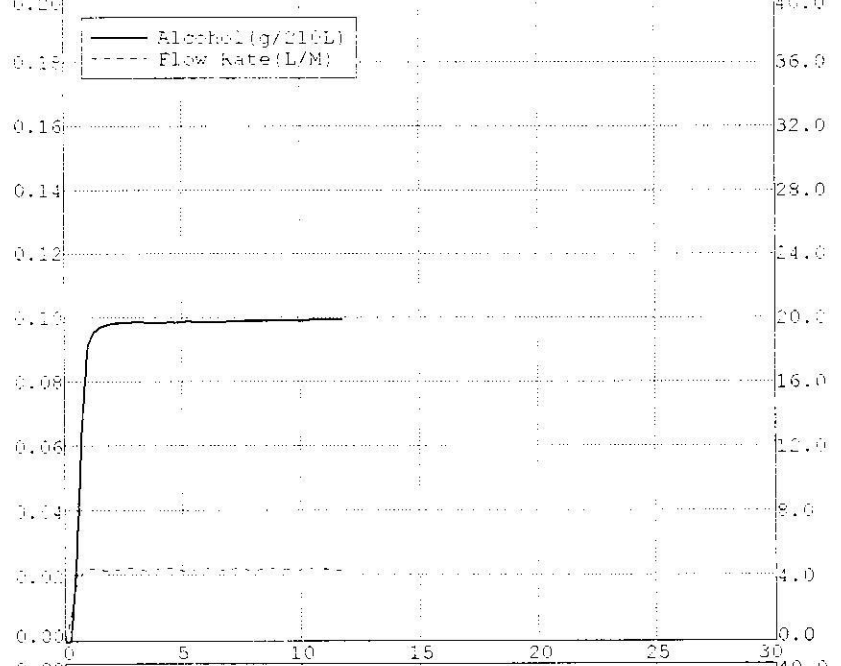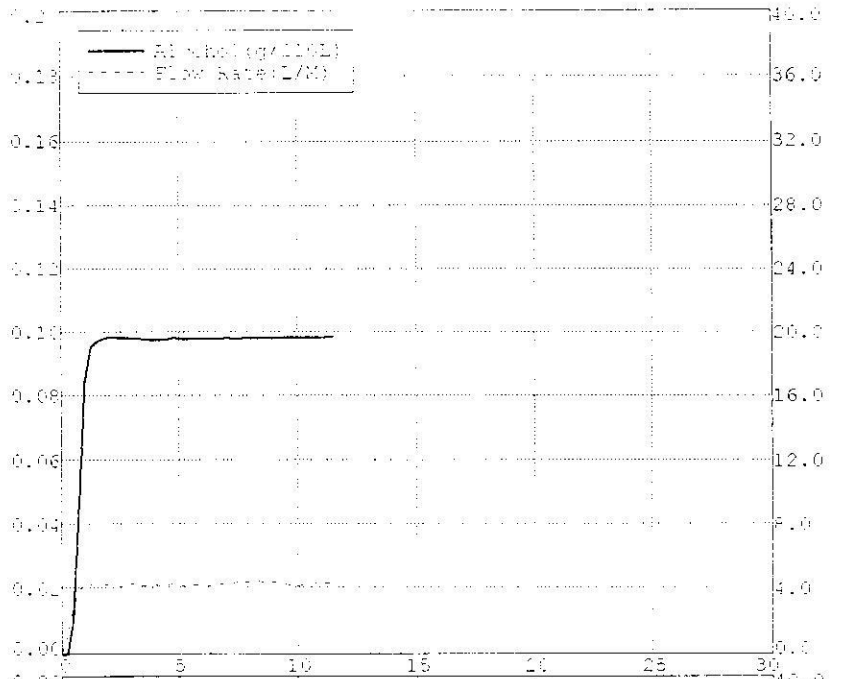

614