

SOLUTION CHANGE




SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 05/04/2024

OPERATOR NAME:  
BRANDON KING  
Permit #: 36388  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:45
INTERNAL STANDARD	VERIFIED	01:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:45
BLANK TEST	0.00	01:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:47
BLANK TEST	0.00	01:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:48
BLANK TEST	0.00	01:49

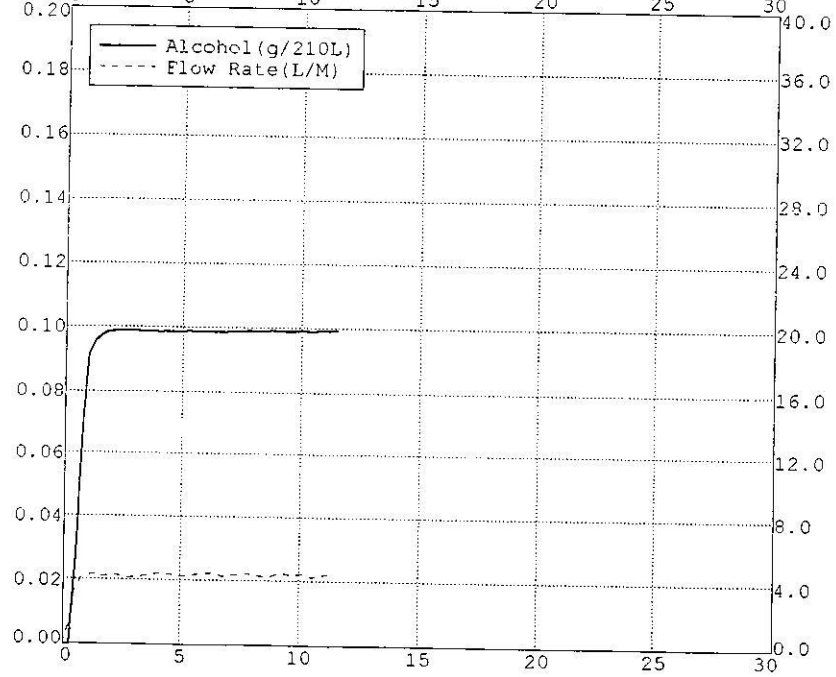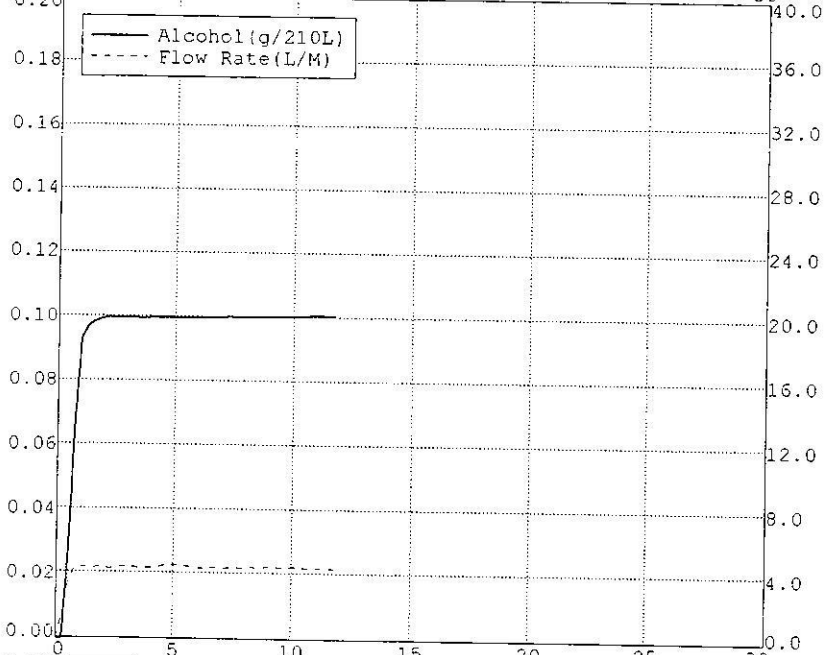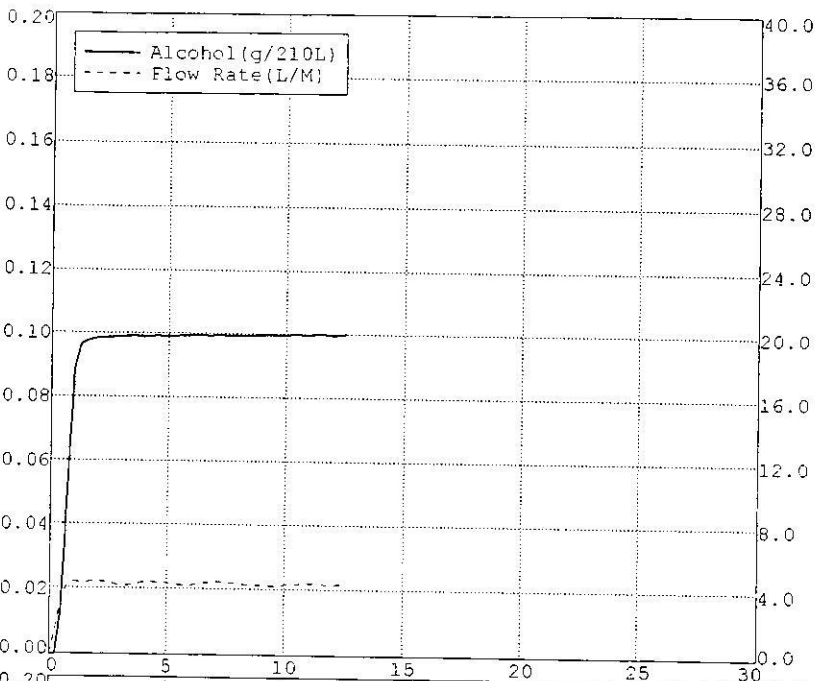

ALCOHOL REFERENCE SOLUTION  
FOR SIMULATOR

24040  
LOT NO.

7/23/24  
EXP DATE

658  
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH  
A PROPERLY OPERATING BREATH SIMULATOR AND  
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL  
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.  
HARRISBURG, PENNSYLVANIA 17111

Rev 1/06

*Handwritten signature/initials*