

SUPERVISOR TEST




SPRING VALLEY VILLAGE
POLICE DEPT
DATAMASTER dmt: 127106

Date: 05/10/2024

OPERATOR NAME:
BRANDON KING
Permit #: 36388
Operator Agency/Dept: SPRING VALLEY PD
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:42
INTERNAL STANDARD	VERIFIED	06:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:43
BLANK TEST	0.00	06:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:44
BLANK TEST	0.00	06:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:45
BLANK TEST	0.00	06:46

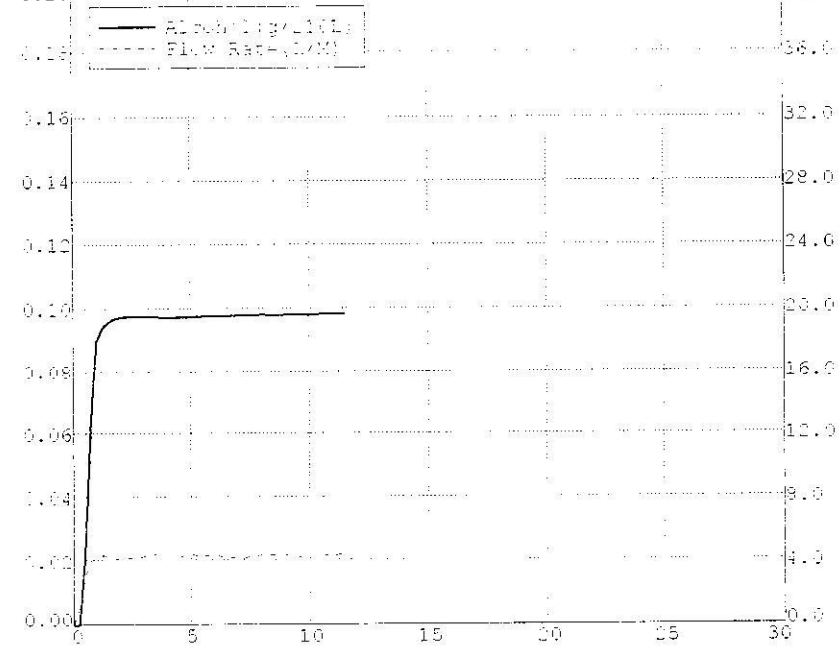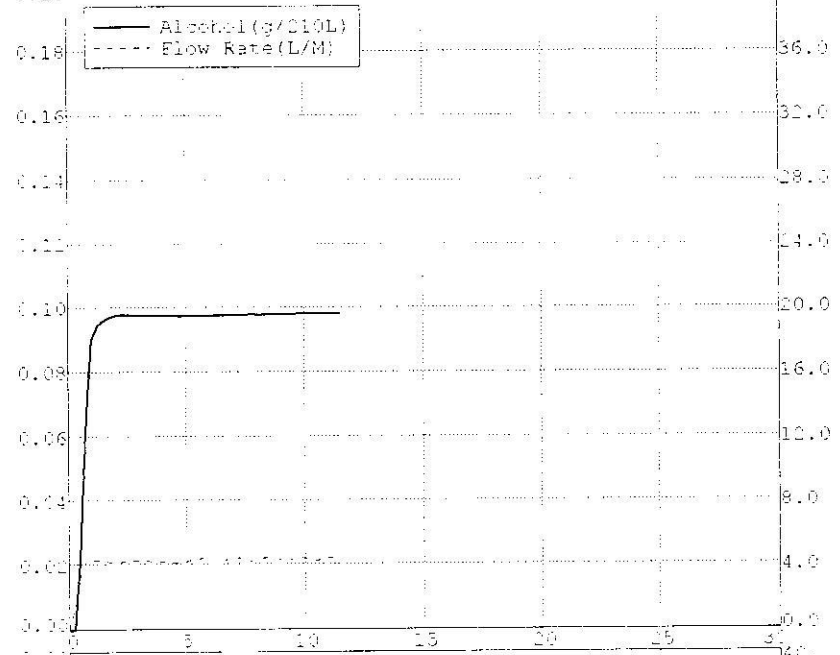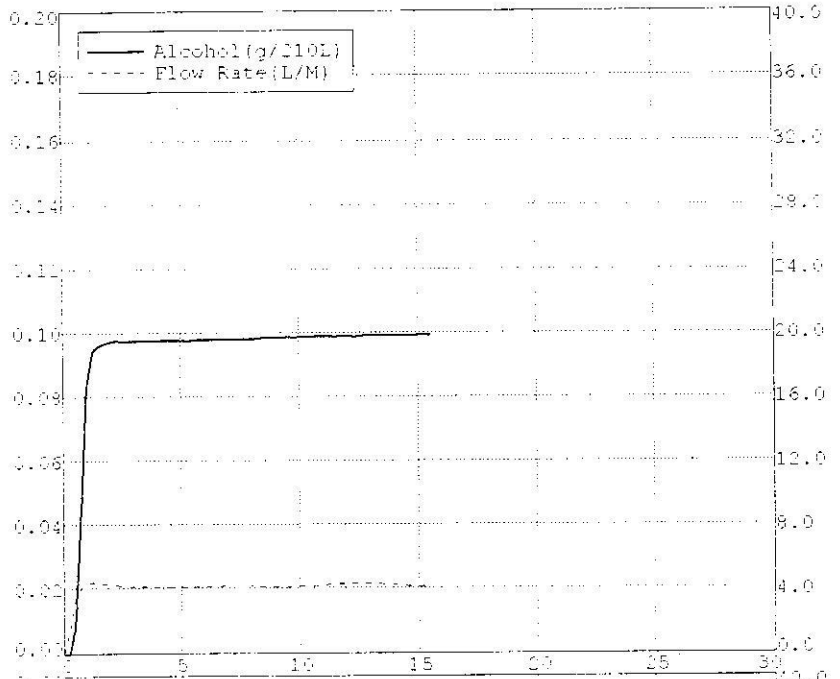

Handwritten signature/initials