

SOLUTION CHANGE



SPRING VALLEY VILLAGE  
POLICE DEPT  
DATAMASTER dmt: 127106

Date: 06/01/2024

OPERATOR NAME:  
JACQUELINE J BLUMFIELD  
Permit #: 38047  
Operator Agency/Dept: SPRING VALLEY PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 08:26 |
| INTERNAL STANDARD       | VERIFIED | 08:26 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 08:26 |
| BLANK TEST              | 0.00     | 08:27 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 08:27 |
| BLANK TEST              | 0.00     | 08:28 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 08:28 |
| BLANK TEST              | 0.00     | 08:29 |

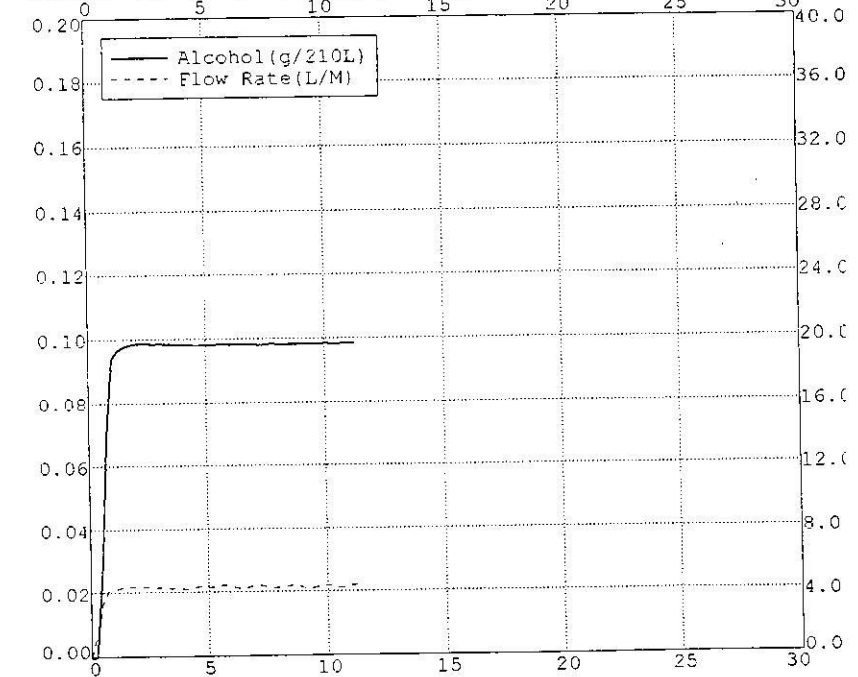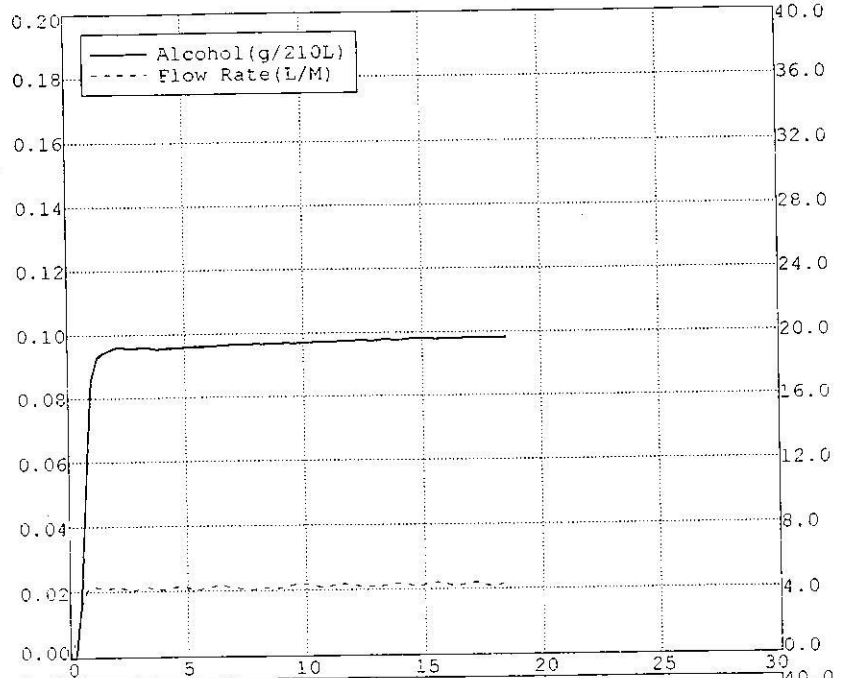

ALCOHOL REFERENCE SOLUTION  
FOR SIMULATOR

24140  
LOT NO.

9/26/24  
EXP. DATE

9/9  
BOT. NO.

WHEN THIS REFERENCE SOLUTION IS USED WITH  
A PROPERLY OPERATING BREATH SIMULATOR AND  
BREATH ALCOHOL ANALYZER, THE SOLUTION WILL  
PROVIDE A VALUE OF 0.10%.

PREPARED AND PACKAGED BY GUTH LABORATORIES, INC.  
HARRISBURG, PENNSYLVANIA 17111

Rev. 1/06